

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052913.D
 Acq On : 01 Feb 2023 18:16
 Operator : JC/MD
 Sample : 01381-14 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	72416	87503	10.26%	1.396%
2	2.562	368	380	398	rVB	179443	289990	34.01%	4.627%
3	2.787	447	450	451	rBV	372	250	0.03%	0.004%
4	2.935	492	496	499	rBV	160	180	0.02%	0.003%
5	2.980	508	510	512	rBV	162	110	0.01%	0.002%
6	3.041	521	529	542	rVB4	2684	4745	0.56%	0.076%
7	3.096	543	546	554	rBB	260	345	0.04%	0.006%
8	3.179	563	572	586	rBB3	1864	3815	0.45%	0.061%
9	3.247	587	593	596	rBB	179	201	0.02%	0.003%
10	3.292	597	607	611	rBB	428	515	0.06%	0.008%
11	3.411	642	644	647	rBB	171	112	0.01%	0.002%
12	3.514	674	676	678	rBV	148	99	0.01%	0.002%
13	3.655	717	720	723	rBB	140	121	0.01%	0.002%
14	3.755	749	751	755	rBB	126	110	0.01%	0.002%
15	4.012	828	831	833	rBB	164	105	0.01%	0.002%
16	4.028	834	836	838	rBV	150	102	0.01%	0.002%
17	4.067	845	848	851	rBV	187	170	0.02%	0.003%
18	4.105	857	860	862	rBB	239	113	0.01%	0.002%
19	4.163	876	878	881	rBB	190	127	0.01%	0.002%
20	4.260	907	908	911	rBV	234	128	0.02%	0.002%
21	4.311	922	924	928	rBV	195	174	0.02%	0.003%
22	4.456	967	969	973	rBB	158	134	0.02%	0.002%
23	4.543	994	996	999	rBB	161	107	0.01%	0.002%
24	4.623	1009	1021	1058	rBV3	55527	188923	22.16%	3.014%
25	4.890	1101	1104	1105	rBV	152	103	0.01%	0.002%
26	4.980	1130	1132	1135	rBV	171	142	0.02%	0.002%
27	5.057	1140	1156	1180	rBV	170548	375134	44.00%	5.985%
28	5.182	1192	1195	1196	rBV	218	139	0.02%	0.002%
29	5.234	1206	1211	1213	rBB	165	158	0.02%	0.003%
30	5.263	1217	1220	1222	rBB	177	119	0.01%	0.002%
31	5.507	1294	1296	1299	rBB	194	119	0.01%	0.002%
32	5.555	1309	1311	1313	rBV	173	116	0.01%	0.002%
33	5.584	1318	1320	1323	rBV	160	135	0.02%	0.002%
34	5.626	1331	1333	1335	rBB	263	102	0.01%	0.002%
35	5.719	1339	1362	1386	rBV3	311300	852549	100.00%	13.602%
36	5.957	1434	1436	1439	rBB3	208	107	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052913.D
 Acq On : 01 Feb 2023 18:16
 Operator : JC/MD
 Sample : 01381-14 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.002	1448	1450	1453	rBB	184	115	0.01%	0.002%
38	6.038	1458	1461	1464	rBB	275	168	0.02%	0.003%
39	6.112	1481	1484	1487	rBV	157	150	0.02%	0.002%
40	6.179	1503	1505	1508	rBV	228	134	0.02%	0.002%
41	6.243	1511	1525	1548	rBV	271625	505067	59.24%	8.058%
42	6.395	1571	1572	1574	rBV	226	109	0.01%	0.002%
43	6.481	1597	1599	1601	rBB	347	132	0.02%	0.002%
44	6.539	1606	1617	1631	rBB4	19933	36764	4.31%	0.587%
45	6.607	1632	1638	1639	rBV2	297	311	0.04%	0.005%
46	6.684	1649	1662	1686	rBV	206716	392938	46.09%	6.269%
47	6.909	1730	1732	1735	rBB	161	106	0.01%	0.002%
48	6.951	1743	1745	1749	rBB	152	118	0.01%	0.002%
49	7.063	1777	1780	1782	rBB	166	110	0.01%	0.002%
50	7.160	1807	1810	1811	rBV	227	118	0.01%	0.002%
51	7.356	1867	1871	1874	rBB	182	180	0.02%	0.003%
52	7.407	1885	1887	1889	rBB	204	102	0.01%	0.002%
53	7.562	1922	1935	1949	rBV	91311	158796	18.63%	2.534%
54	7.690	1969	1975	1978	rBV2	770	806	0.09%	0.013%
55	7.893	2025	2038	2059	rBV	359371	612196	71.81%	9.767%
56	8.108	2103	2105	2108	rBB	246	123	0.01%	0.002%
57	8.176	2115	2126	2144	rBV	65964	112138	13.15%	1.789%
58	8.311	2166	2168	2171	rBB	203	129	0.02%	0.002%
59	8.449	2207	2211	2212	rBV	417	285	0.03%	0.005%
60	8.542	2237	2240	2242	rBV	133	114	0.01%	0.002%
61	8.581	2250	2252	2257	rBB	163	134	0.02%	0.002%
62	8.639	2258	2270	2304	rBV2	134856	285648	33.51%	4.557%
63	8.806	2318	2322	2325	rBV2	303	300	0.04%	0.005%
64	9.009	2381	2385	2389	rBB	170	183	0.02%	0.003%
65	9.063	2399	2402	2405	rBB	223	166	0.02%	0.003%
66	9.083	2405	2408	2410	rBB	164	107	0.01%	0.002%
67	9.153	2428	2430	2433	rBV	150	122	0.01%	0.002%
68	9.279	2465	2469	2472	rBB	206	182	0.02%	0.003%
69	9.308	2475	2478	2480	rBB	154	104	0.01%	0.002%
70	9.337	2485	2487	2489	rBV	147	109	0.01%	0.002%
71	9.414	2498	2511	2534	rBV	339845	610945	71.66%	9.747%
72	9.587	2561	2565	2567	rBB	139	121	0.01%	0.002%
73	9.642	2578	2582	2586	rBB	179	199	0.02%	0.003%
74	9.748	2612	2615	2620	rBB	195	192	0.02%	0.003%
75	9.780	2623	2625	2629	rBB	155	119	0.01%	0.002%
76	9.841	2640	2644	2648	rBB	198	217	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052913.D
 Acq On : 01 Feb 2023 18:16
 Operator : JC/MD
 Sample : 01381-14 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.095	2720	2723	2725	rBV	149	133	0.02%	0.002%
78	10.124	2730	2732	2735	rBB	142	100	0.01%	0.002%
79	10.163	2741	2744	2746	rBV	158	132	0.02%	0.002%
80	10.205	2755	2757	2759	rBV	154	109	0.01%	0.002%
81	10.365	2803	2807	2810	rBB	199	185	0.02%	0.003%
82	10.407	2817	2820	2822	rBB	201	127	0.01%	0.002%
83	10.436	2827	2829	2830	rBV	197	100	0.01%	0.002%
84	10.475	2838	2841	2844	rBB	202	149	0.02%	0.002%
85	10.513	2848	2853	2861	rBB	229	421	0.05%	0.007%
86	10.706	2908	2913	2915	rBV	197	211	0.02%	0.003%
87	10.755	2915	2928	2942	rVV	244783	393705	46.18%	6.281%
88	10.864	2958	2962	2963	rBV	265	183	0.02%	0.003%
89	10.980	2994	2998	3001	rBV	268	250	0.03%	0.004%
90	11.021	3008	3011	3017	rBV	281	287	0.03%	0.005%
91	11.092	3025	3033	3035	rBV	221	285	0.03%	0.005%
92	11.195	3061	3065	3068	rBV	192	208	0.02%	0.003%
93	11.298	3092	3097	3102	rBV	267	324	0.04%	0.005%
94	11.542	3169	3173	3174	rBV	166	144	0.02%	0.002%
95	11.623	3195	3198	3202	rBV	197	207	0.02%	0.003%
96	11.809	3244	3256	3278	rBV	365065	598782	70.23%	9.553%
97	12.189	3361	3374	3400	rBV2	401903	744148	87.29%	11.873%
98	12.816	3566	3569	3571	rBV2	304	212	0.02%	0.003%
99	12.848	3577	3579	3580	rBV2	283	111	0.01%	0.002%
100	13.880	3898	3900	3903	rVB	350	135	0.02%	0.002%




Sum of corrected areas: 6267807

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052913.D
Acq On : 01 Feb 2023 18:16
Operator : JC/MD
Sample : 01381-14 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

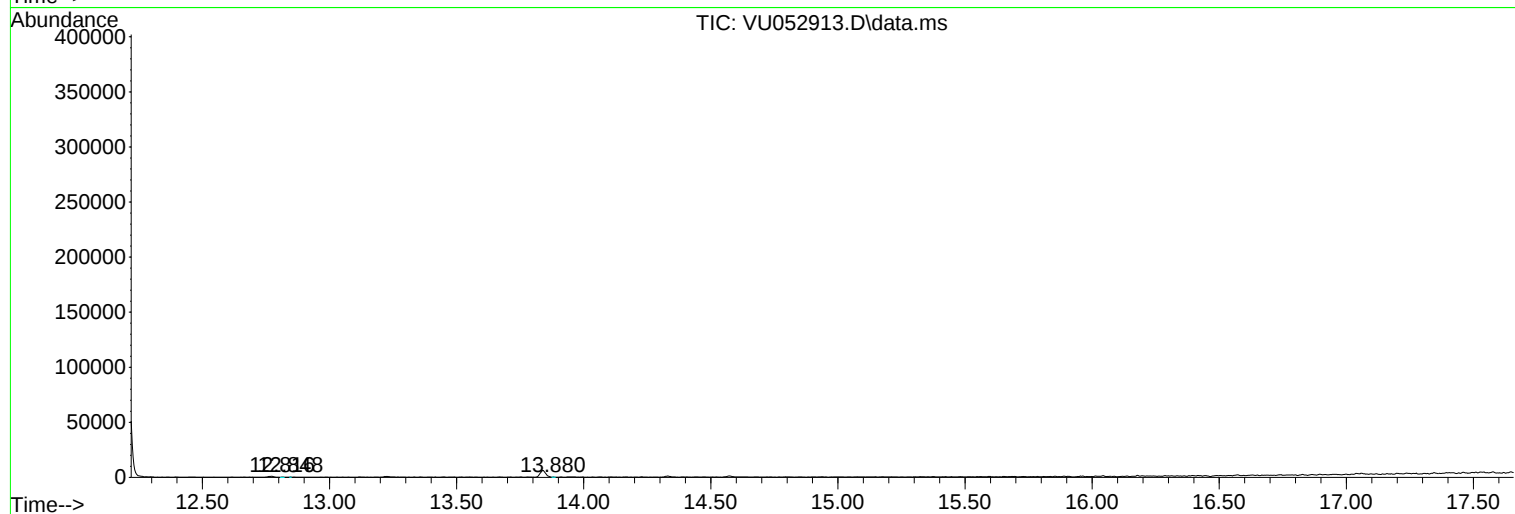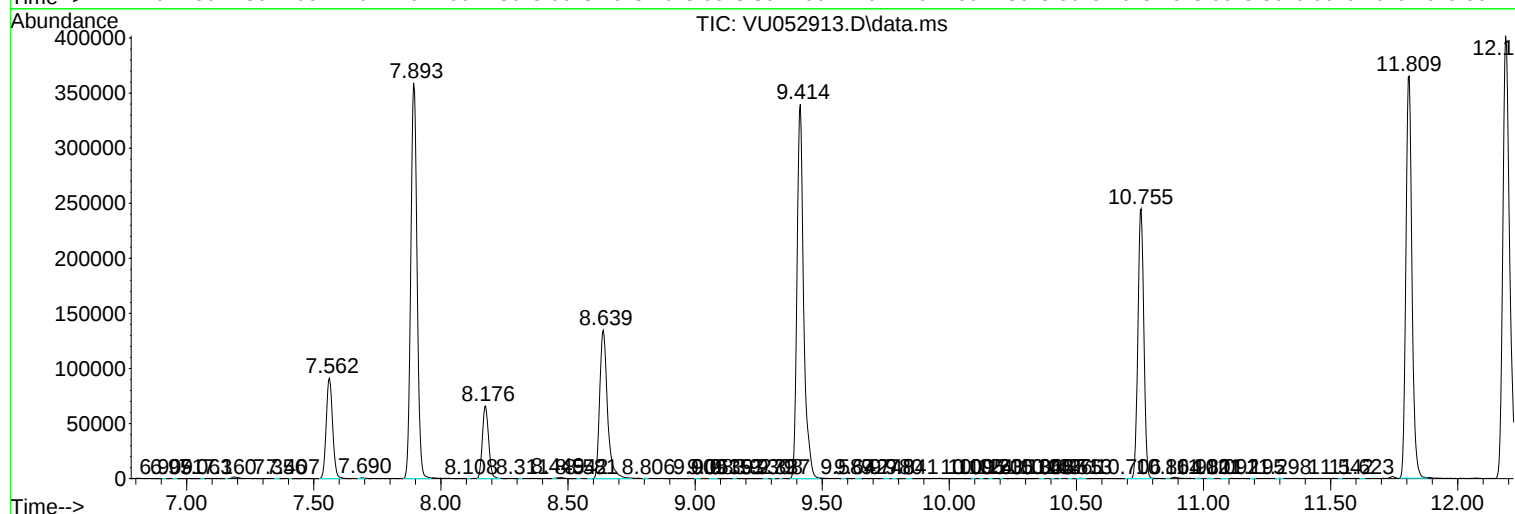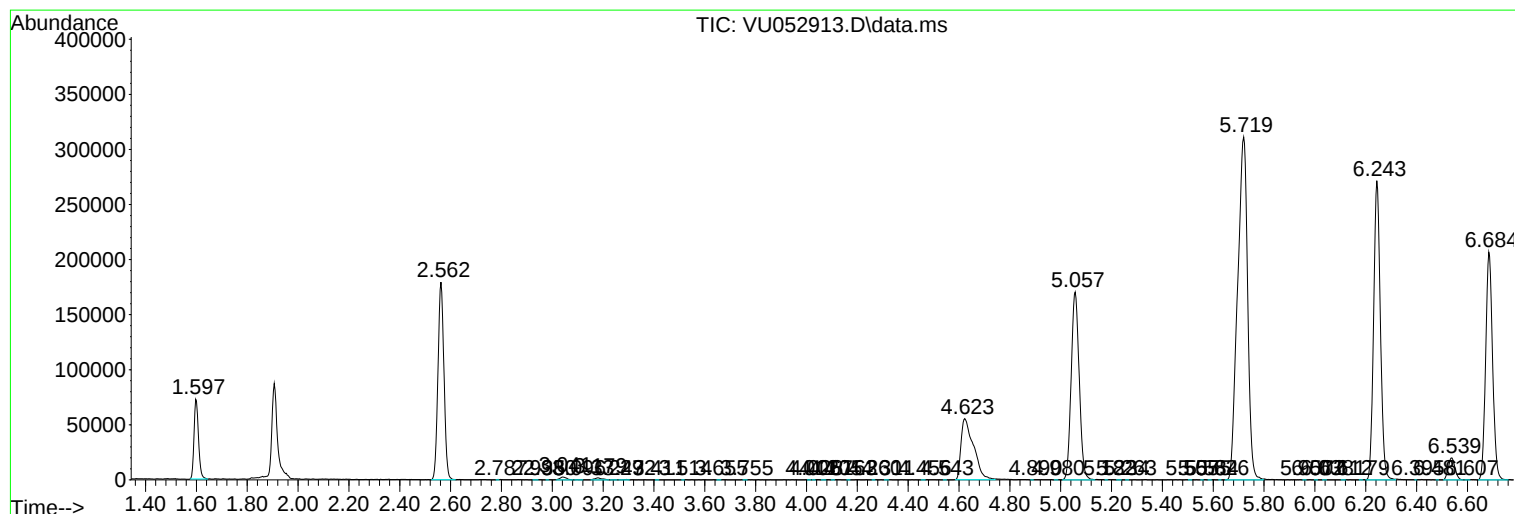

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052913.D
Acq On : 01 Feb 2023 18:16
Operator : JC/MD
Sample : 01381-14 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052913.D
Acq On : 01 Feb 2023 18:16
Operator : JC/MD
Sample : 01381-14 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------