

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052914.D
 Acq On : 01 Feb 2023 18:39
 Operator : JC/MD
 Sample : 01381-12 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rBV	69216	87072	11.51%	1.471%
2	1.903	168	175	191	rBV	81615	118311	15.64%	1.999%
3	2.559	367	379	399	rBV	182378	293078	38.74%	4.951%
4	2.748	432	438	442	rBV	249	348	0.05%	0.006%
5	2.806	452	456	458	rBV	147	143	0.02%	0.002%
6	2.883	477	480	483	rBB	160	128	0.02%	0.002%
7	2.938	494	497	501	rBV	241	222	0.03%	0.004%
8	3.038	521	528	540	rBB4	3253	6122	0.81%	0.103%
9	3.089	541	544	547	rBB	284	201	0.03%	0.003%
10	3.182	564	573	581	rVV4	1645	2742	0.36%	0.046%
11	3.314	608	614	615	rBV	556	443	0.06%	0.007%
12	3.433	647	651	653	rBB	199	153	0.02%	0.003%
13	3.928	803	805	808	rBV	185	141	0.02%	0.002%
14	4.623	1010	1021	1048	rBV2	42458	117250	15.50%	1.981%
15	4.993	1134	1136	1140	rBB	174	145	0.02%	0.002%
16	5.057	1140	1156	1182	rBV	146346	319982	42.29%	5.406%
17	5.369	1251	1253	1257	rBB	179	142	0.02%	0.002%
18	5.719	1341	1362	1384	rBV2	277075	756585	100.00%	12.782%
19	5.838	1397	1399	1403	rVB	402	234	0.03%	0.004%
20	6.243	1511	1525	1552	rBV	245616	462093	61.08%	7.806%
21	6.356	1557	1560	1563	rVB2	289	181	0.02%	0.003%
22	6.536	1606	1616	1626	rVV6	2980	5518	0.73%	0.093%
23	6.594	1629	1634	1636	rBV	390	285	0.04%	0.005%
24	6.684	1648	1662	1679	rBV	200401	385494	50.95%	6.512%
25	6.800	1696	1698	1700	rBV	305	198	0.03%	0.003%
26	6.813	1700	1702	1707	rVB2	506	324	0.04%	0.005%
27	6.877	1719	1722	1726	rBB	183	178	0.02%	0.003%
28	7.009	1760	1763	1766	rBV	192	176	0.02%	0.003%
29	7.076	1780	1784	1786	rBV	131	139	0.02%	0.002%
30	7.182	1812	1817	1819	rBV2	1877	1562	0.21%	0.026%
31	7.292	1849	1851	1856	rBB	176	163	0.02%	0.003%
32	7.353	1867	1870	1874	rBB2	251	205	0.03%	0.003%
33	7.562	1923	1935	1953	rBV	101422	176316	23.30%	2.979%
34	7.629	1953	1956	1961	rVB2	400	378	0.05%	0.006%
35	7.681	1969	1972	1974	rBV3	409	292	0.04%	0.005%
36	7.771	1997	2000	2004	rBV	207	209	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052914.D
 Acq On : 01 Feb 2023 18:39
 Operator : JC/MD
 Sample : 01381-12 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	7.893	2025	2038	2059	rBV	391339	675167	89.24%	11.406%
38	8.060	2088	2090	2095	rVB2	207	143	0.02%	0.002%
39	8.112	2105	2106	2110	rVB	224	136	0.02%	0.002%
40	8.176	2114	2126	2142	rBV	74000	125245	16.55%	2.116%
41	8.272	2153	2156	2158	rBV	224	136	0.02%	0.002%
42	8.317	2165	2170	2173	rVV2	335	256	0.03%	0.004%
43	8.420	2199	2202	2207	rBV2	302	239	0.03%	0.004%
44	8.459	2211	2214	2216	rBV	435	272	0.04%	0.005%
45	8.645	2259	2272	2304	rBV3	150996	327898	43.34%	5.539%
46	8.800	2317	2320	2325	rVV2	504	318	0.04%	0.005%
47	8.835	2328	2331	2333	rVV	210	155	0.02%	0.003%
48	8.864	2337	2340	2345	rVB	299	304	0.04%	0.005%
49	9.137	2420	2425	2428	rBV	154	194	0.03%	0.003%
50	9.211	2444	2448	2451	rBB	149	148	0.02%	0.003%
51	9.356	2490	2493	2495	rBV	168	137	0.02%	0.002%
52	9.414	2499	2511	2529	rBV	339348	559565	73.96%	9.453%
53	9.520	2540	2544	2545	rVB	261	164	0.02%	0.003%
54	9.555	2552	2555	2557	rBV	277	175	0.02%	0.003%
55	9.703	2594	2601	2603	rBV	169	212	0.03%	0.004%
56	9.829	2634	2640	2642	rBV	157	217	0.03%	0.004%
57	9.935	2671	2673	2677	rVB	250	161	0.02%	0.003%
58	10.034	2700	2704	2706	rBV	149	145	0.02%	0.002%
59	10.147	2736	2739	2742	rBB	213	163	0.02%	0.003%
60	10.369	2803	2808	2810	rBB	267	190	0.03%	0.003%
61	10.388	2811	2814	2817	rBB	196	148	0.02%	0.003%
62	10.414	2818	2822	2824	rBB	197	150	0.02%	0.003%
63	10.520	2852	2855	2858	rBB	189	148	0.02%	0.003%
64	10.755	2916	2928	2943	rBV	237031	388690	51.37%	6.566%
65	10.861	2959	2961	2964	rBB	246	142	0.02%	0.002%
66	10.890	2965	2970	2975	rBB2	676	710	0.09%	0.012%
67	11.034	3012	3015	3017	rBV	158	132	0.02%	0.002%
68	11.102	3034	3036	3038	rBV	182	129	0.02%	0.002%
69	11.134	3043	3046	3048	rBV	242	183	0.02%	0.003%
70	11.192	3060	3064	3067	rBV	261	249	0.03%	0.004%
71	11.433	3136	3139	3143	rBB	232	203	0.03%	0.003%
72	11.484	3150	3155	3158	rBV	186	235	0.03%	0.004%
73	11.677	3211	3215	3222	rBB	298	247	0.03%	0.004%
74	11.748	3234	3237	3240	rBB2	378	281	0.04%	0.005%
75	11.809	3243	3256	3278	rVV	335789	531401	70.24%	8.977%
76	11.899	3282	3284	3288	rVB2	405	204	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052914.D
 Acq On : 01 Feb 2023 18:39
 Operator : JC/MD
 Sample : 01381-12 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.941	3293	3297	3301	rVB2	285	278	0.04%	0.005%
78	11.986	3306	3311	3314	rBV	177	187	0.02%	0.003%
79	12.060	3328	3334	3338	rBB	154	208	0.03%	0.004%
80	12.115	3345	3351	3354	rBV	205	287	0.04%	0.005%
81	12.189	3362	3374	3391	rBV	345036	558187	73.78%	9.430%
82	12.327	3413	3417	3422	rBV	211	153	0.02%	0.003%
83	12.401	3437	3440	3443	rBV	175	164	0.02%	0.003%
84	12.475	3459	3463	3465	rVV	280	221	0.03%	0.004%
85	12.594	3497	3500	3504	rBV	160	177	0.02%	0.003%
86	12.687	3526	3529	3531	rBV	240	135	0.02%	0.002%
87	12.774	3549	3556	3560	rVV	489	603	0.08%	0.010%
88	12.889	3588	3592	3597	rBV	235	333	0.04%	0.006%
89	13.240	3699	3701	3703	rVB	276	129	0.02%	0.002%
90	13.262	3704	3708	3710	rBV	260	227	0.03%	0.004%
91	13.404	3751	3752	3755	rBV	245	159	0.02%	0.003%
92	13.523	3786	3789	3796	rBV	125	135	0.02%	0.002%
93	13.841	3877	3888	3894	rBV5	2223	3547	0.47%	0.060%
94	14.066	3955	3958	3964	rBV2	231	185	0.02%	0.003%
95	14.295	4027	4029	4033	rVB	291	162	0.02%	0.003%
96	14.336	4037	4042	4046	rVB4	601	743	0.10%	0.013%
97	14.369	4046	4052	4054	rBV2	277	278	0.04%	0.005%
98	14.770	4172	4177	4180	rBV2	314	310	0.04%	0.005%
99	14.983	4241	4243	4248	rBV	338	227	0.03%	0.004%
100	15.095	4275	4278	4279	rBV	282	180	0.02%	0.003%




Sum of corrected areas: 5919360

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052914.D
Acq On : 01 Feb 2023 18:39
Operator : JC/MD
Sample : 01381-12 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

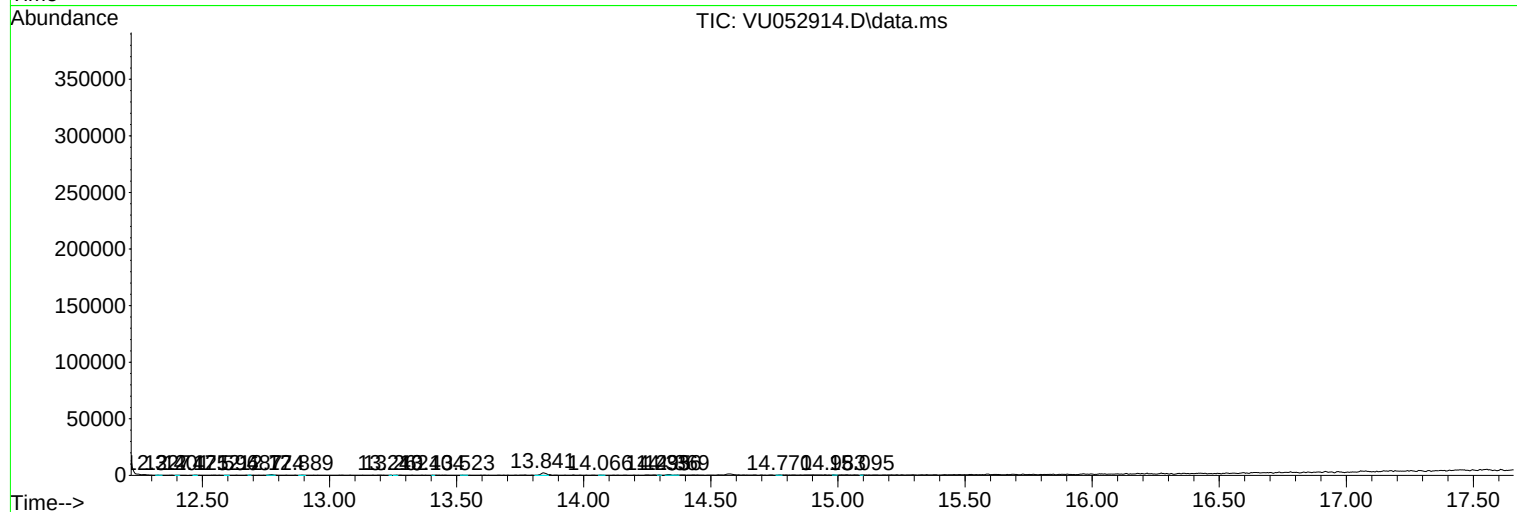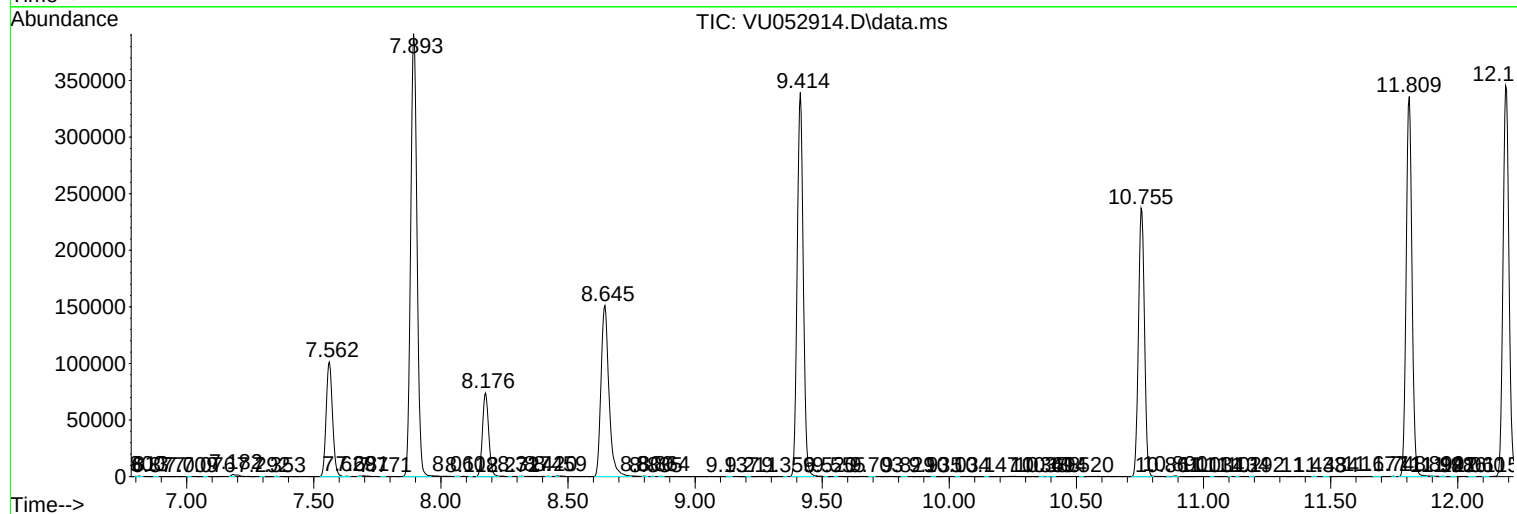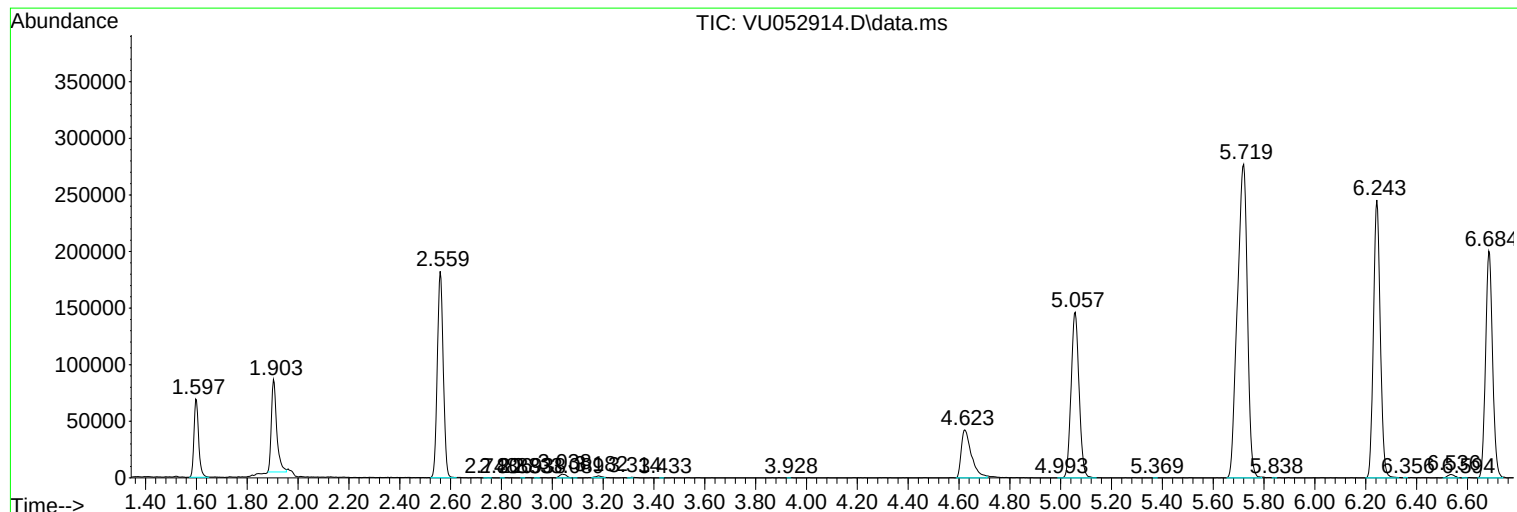

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052914.D
Acq On : 01 Feb 2023 18:39
Operator : JC/MD
Sample : 01381-12 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052914.D
Acq On : 01 Feb 2023 18:39
Operator : JC/MD
Sample : 01381-12 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------