

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052915.D
 Acq On : 01 Feb 2023 19:03
 Operator : JC/MD
 Sample : 01381-11 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	70976	90249	11.71%	1.534%
2	2.559	367	379	396	rBV	162512	262365	34.05%	4.458%
3	2.710	424	426	428	rBB	249	117	0.02%	0.002%
4	2.742	433	436	439	rBV	165	172	0.02%	0.003%
5	2.781	446	448	452	rVB	380	275	0.04%	0.005%
6	2.806	453	456	460	rBB	145	142	0.02%	0.002%
7	2.874	474	477	478	rBV	177	122	0.02%	0.002%
8	2.909	486	488	490	rBB	243	118	0.02%	0.002%
9	2.938	495	497	501	rBB	168	135	0.02%	0.002%
10	2.974	505	508	510	rBB	161	104	0.01%	0.002%
11	3.041	520	529	540	rBV4	2793	5290	0.69%	0.090%
12	3.179	561	572	589	rBB	1876	4082	0.53%	0.069%
13	3.398	637	640	644	rBB	142	140	0.02%	0.002%
14	3.440	650	653	655	rBV	190	144	0.02%	0.002%
15	3.636	711	714	717	rBB	163	109	0.01%	0.002%
16	3.864	783	785	788	rBB	151	100	0.01%	0.002%
17	4.218	892	895	897	rBB	193	121	0.02%	0.002%
18	4.623	1010	1021	1047	rBV	43290	119049	15.45%	2.023%
19	4.842	1087	1089	1092	rBB	166	110	0.01%	0.002%
20	4.906	1107	1109	1113	rBB	184	135	0.02%	0.002%
21	5.057	1140	1156	1181	rBV2	147109	325156	42.20%	5.525%
22	5.292	1227	1229	1231	rBB	245	110	0.01%	0.002%
23	5.719	1341	1362	1384	rBV2	284500	770484	100.00%	13.093%
24	6.243	1510	1525	1543	rBV	280100	520147	67.51%	8.839%
25	6.530	1607	1614	1624	rBB7	1754	3368	0.44%	0.057%
26	6.584	1628	1631	1632	rBV	229	124	0.02%	0.002%
27	6.616	1639	1641	1643	rBB	237	113	0.01%	0.002%
28	6.684	1649	1662	1681	rBV	202669	388923	50.48%	6.609%
29	6.780	1688	1692	1694	rBV	148	125	0.02%	0.002%
30	7.099	1789	1791	1794	rBB	190	122	0.02%	0.002%
31	7.137	1799	1803	1806	rBB	152	157	0.02%	0.003%
32	7.186	1807	1818	1820	rBV2	1599	1942	0.25%	0.033%
33	7.266	1841	1843	1846	rBB	258	137	0.02%	0.002%
34	7.292	1846	1851	1854	rBV2	274	268	0.03%	0.005%
35	7.382	1877	1879	1881	rBV	170	106	0.01%	0.002%
36	7.481	1906	1910	1913	rBB	286	209	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052915.D
 Acq On : 01 Feb 2023 19:03
 Operator : JC/MD
 Sample : 01381-11 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	7.562	1923	1935	1952	rVV2	109139	191530	24.86%	3.255%
38	7.694	1972	1976	1977	rBV	582	368	0.05%	0.006%
39	7.809	2010	2012	2015	rBB	176	119	0.02%	0.002%
40	7.893	2025	2038	2060	rVV	415783	703138	91.26%	11.949%
41	8.176	2115	2126	2142	rVV	73166	121926	15.82%	2.072%
42	8.385	2188	2191	2194	rBB	334	131	0.02%	0.002%
43	8.407	2196	2198	2201	rBB	209	101	0.01%	0.002%
44	8.462	2204	2215	2216	rBV2	582	720	0.09%	0.012%
45	8.546	2239	2241	2244	rBV	161	132	0.02%	0.002%
46	8.591	2252	2255	2257	rBB	158	105	0.01%	0.002%
47	8.642	2258	2271	2301	rBV2	132563	285473	37.05%	4.851%
48	8.896	2345	2350	2351	rBV	163	164	0.02%	0.003%
49	8.919	2354	2357	2361	rBB	168	157	0.02%	0.003%
50	8.944	2362	2365	2371	rBB	188	230	0.03%	0.004%
51	8.970	2371	2373	2375	rBV	164	114	0.01%	0.002%
52	9.028	2389	2391	2394	rBB	177	110	0.01%	0.002%
53	9.073	2403	2405	2408	rBB	145	101	0.01%	0.002%
54	9.095	2409	2412	2414	rBB	192	123	0.02%	0.002%
55	9.192	2438	2442	2445	rBB	124	108	0.01%	0.002%
56	9.224	2450	2452	2455	rBB	173	106	0.01%	0.002%
57	9.314	2477	2480	2483	rBB	179	140	0.02%	0.002%
58	9.340	2484	2488	2489	rBV	232	113	0.01%	0.002%
59	9.414	2498	2511	2529	rBV	337450	566391	73.51%	9.625%
60	9.623	2573	2576	2579	rBB	225	158	0.02%	0.003%
61	9.761	2616	2619	2621	rBB	193	117	0.02%	0.002%
62	9.809	2631	2634	2636	rBV	150	104	0.01%	0.002%
63	9.848	2641	2646	2648	rBB	161	160	0.02%	0.003%
64	10.034	2702	2704	2708	rBV	139	144	0.02%	0.002%
65	10.192	2749	2753	2756	rBB	183	144	0.02%	0.002%
66	10.237	2761	2767	2771	rBB	303	308	0.04%	0.005%
67	10.263	2772	2775	2778	rBB	160	102	0.01%	0.002%
68	10.337	2794	2798	2800	rBV	139	128	0.02%	0.002%
69	10.385	2811	2813	2817	rBV	330	282	0.04%	0.005%
70	10.484	2842	2844	2847	rBV	149	121	0.02%	0.002%
71	10.513	2851	2853	2856	rBB	147	102	0.01%	0.002%
72	10.755	2914	2928	2946	rBV	249403	392690	50.97%	6.673%
73	10.883	2961	2968	2969	rBV2	491	526	0.07%	0.009%
74	10.983	2997	2999	3002	rBV	148	120	0.02%	0.002%
75	11.018	3007	3010	3015	rBV	195	223	0.03%	0.004%
76	11.201	3065	3067	3070	rBV	134	111	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
 Data File : VU052915.D
 Acq On : 01 Feb 2023 19:03
 Operator : JC/MD
 Sample : 01381-11 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.279	3089	3091	3094	rBV	150	119	0.02%	0.002%
78	11.398	3124	3128	3133	rBV	173	241	0.03%	0.004%
79	11.507	3159	3162	3164	rBB	181	122	0.02%	0.002%
80	11.523	3165	3167	3171	rBV	229	187	0.02%	0.003%
81	11.610	3192	3194	3196	rBV	163	110	0.01%	0.002%
82	11.809	3243	3256	3273	rBV	340338	532616	69.13%	9.051%
83	11.983	3308	3310	3313	rBV	131	111	0.01%	0.002%
84	12.021	3319	3322	3326	rBB	153	150	0.02%	0.003%
85	12.044	3326	3329	3332	rBV	282	181	0.02%	0.003%
86	12.099	3344	3346	3349	rBB	278	167	0.02%	0.003%
87	12.124	3350	3354	3357	rBV	190	201	0.03%	0.003%
88	12.189	3361	3374	3394	rBV	356460	585444	75.98%	9.949%
89	12.365	3427	3429	3432	rBB	195	124	0.02%	0.002%
90	12.388	3432	3436	3441	rBB	168	204	0.03%	0.003%
91	12.430	3444	3449	3452	rBV	169	235	0.03%	0.004%
92	12.504	3468	3472	3474	rBV	178	159	0.02%	0.003%
93	12.597	3496	3501	3505	rBV	182	248	0.03%	0.004%
94	12.754	3546	3550	3552	rBV2	576	444	0.06%	0.008%
95	12.992	3620	3624	3629	rBV2	287	352	0.05%	0.006%
96	13.070	3643	3648	3652	rBV	292	303	0.04%	0.005%
97	13.256	3703	3706	3708	rBV	260	143	0.02%	0.002%
98	13.353	3731	3736	3740	rBV	300	416	0.05%	0.007%
99	13.481	3770	3776	3777	rBV	310	256	0.03%	0.004%
100	13.832	3882	3885	3886	rBV2	753	424	0.06%	0.007%




Sum of corrected areas: 5884667

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052915.D
Acq On : 01 Feb 2023 19:03
Operator : JC/MD
Sample : 01381-11 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

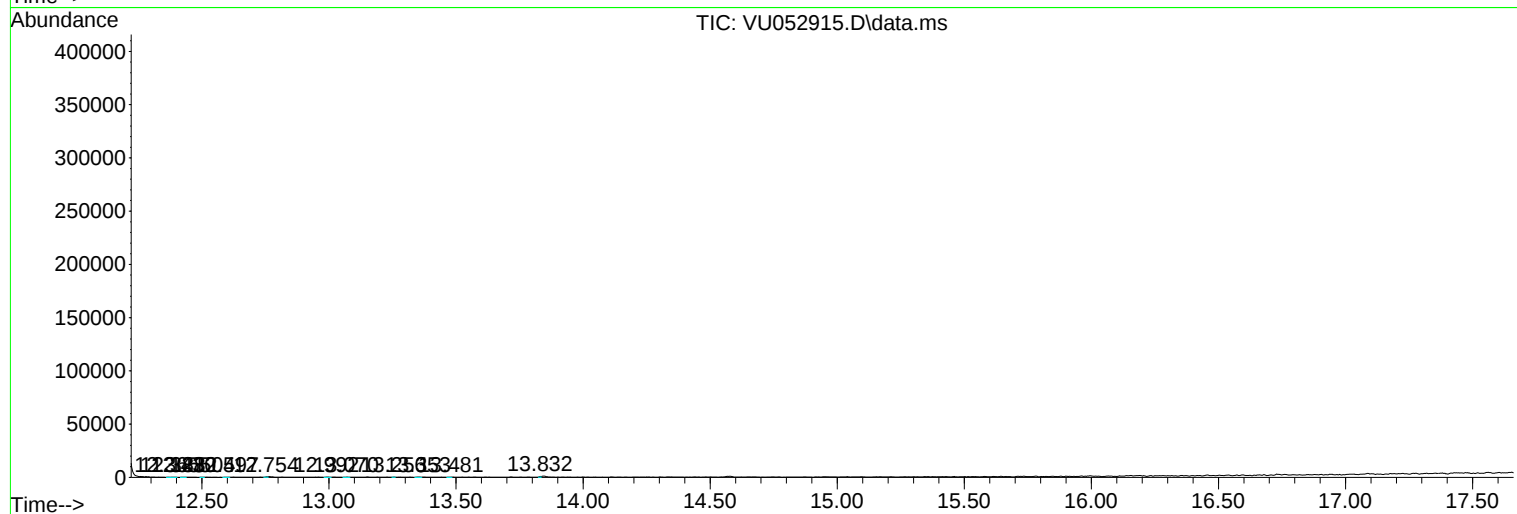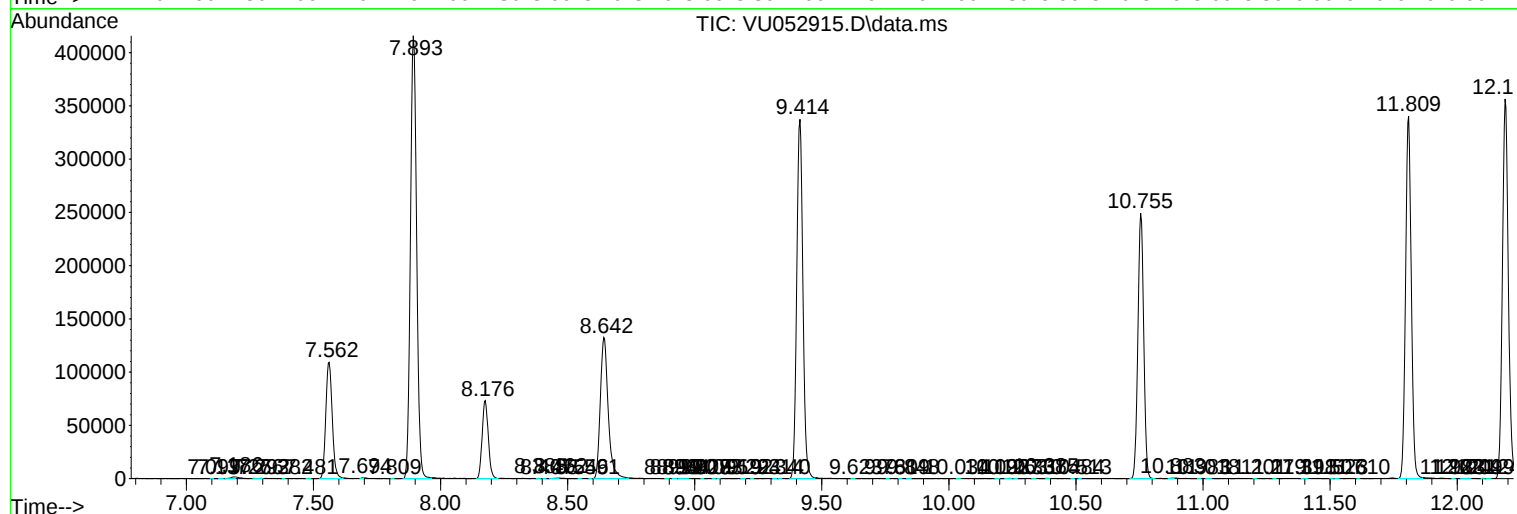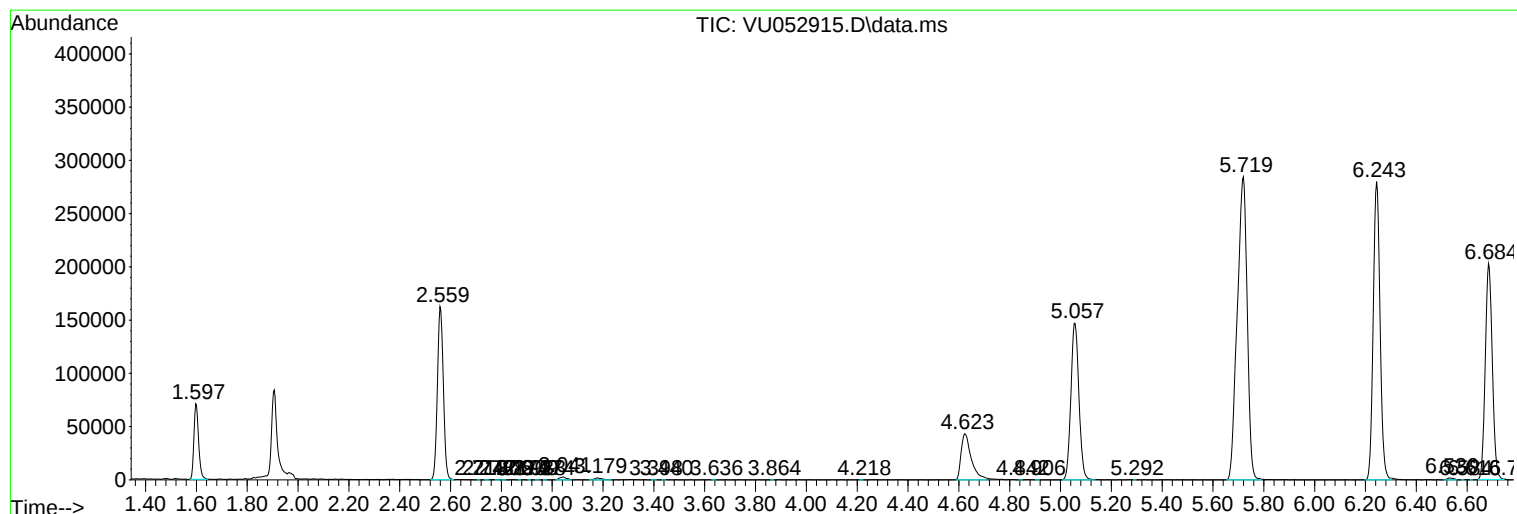

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052915.D
Acq On : 01 Feb 2023 19:03
Operator : JC/MD
Sample : 01381-11 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052915.D
Acq On : 01 Feb 2023 19:03
Operator : JC/MD
Sample : 01381-11 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------