


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020123\
Data File : VU052895.D
Acq On : 01 Feb 2023 10:35
Operator : JC/MD
Sample : BFB156
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB156

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Title : VOC Analysis
Last Update : Fri Feb 03 00:24:34 2023

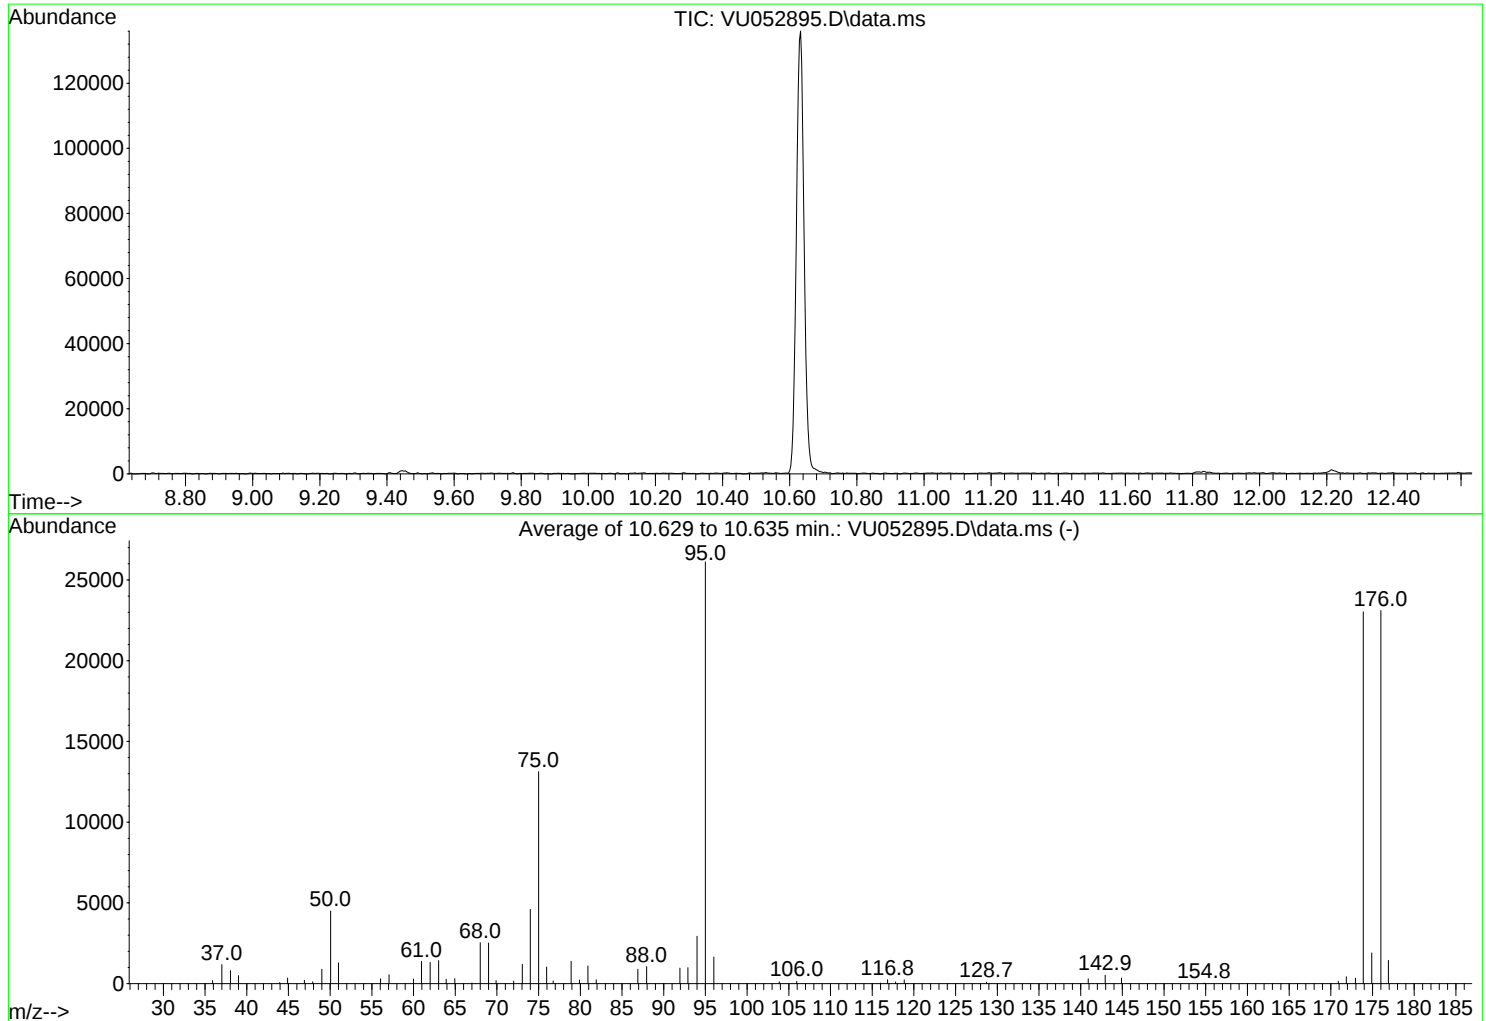

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4503	PASS
75	95	30	80	50.3	13131	PASS
95	95	100	100	100.0	26123	PASS
96	95	5	9	6.3	1641	PASS
173	174	0.00	2	1.4	333	PASS
174	95	50	120	88.1	23027	PASS
175	174	5	9	8.3	1905	PASS
176	174	95	101	100.4	23109	PASS
177	176	5	9	6.2	1433	PASS

m/z	Abundance
43.90	211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	189.0
37.00	1246.0
38.00	857.0
39.00	432.0
44.00	353.0
44.90	361.0
46.90	186.0
47.90	109.0
49.00	892.0
50.10	4567.0
51.00	1288.0
56.00	355.0
57.00	555.0
60.00	288.0
60.90	1417.0
62.00	1242.0
63.00	1383.0
63.90	323.0
65.00	333.0
68.00	2455.0
69.00	2670.0
69.90	204.0
72.00	187.0
73.10	1268.0
74.00	4730.0
75.00	13437.0
76.00	966.0
76.80	186.0
78.90	1352.0
79.90	250.0
80.90	1183.0
81.90	229.0
86.90	979.0
87.90	1103.0
91.90	960.0
92.90	998.0
94.00	2931.0
95.00	26784.0
96.00	1619.0
104.00	104.0
105.90	124.0
116.80	237.0
117.80	179.0
118.80	292.0
128.70	141.0
140.90	295.0
143.00	460.0
144.90	332.0
170.90	161.0
171.80	418.0
172.90	310.0
173.90	22928.0
174.90	1906.0
176.00	22848.0
176.90	1519.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	181.0
37.00	1195.0
38.10	824.0
39.00	500.0
44.10	285.0
44.90	377.0
46.90	216.0
47.90	121.0
49.00	954.0
50.10	4631.0
51.00	1300.0
56.10	300.0
57.10	559.0
60.00	307.0
61.00	1432.0
62.00	1388.0
63.00	1505.0
63.90	300.0
65.00	310.0
68.00	2613.0
69.00	2546.0
69.90	193.0
72.00	162.0
73.00	1250.0
74.00	4746.0
75.00	13497.0
75.90	1052.0
76.70	186.0
78.90	1457.0
79.90	234.0
80.90	1110.0
81.90	250.0
86.90	882.0
88.00	1041.0
91.90	1031.0
92.90	1032.0
94.00	3049.0
95.00	26928.0
96.00	1704.0
103.80	127.0
106.00	152.0
116.00	108.0
116.80	267.0
117.80	162.0
118.80	242.0
128.70	136.0
140.90	309.0
143.00	550.0
144.90	369.0
170.90	147.0
171.90	432.0
172.90	336.0
173.90	23808.0
174.90	1987.0
176.00	23776.0
176.90	1461.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	185.0
37.00	1110.0
38.10	729.0
39.00	542.0
44.00	213.0
44.90	304.0
46.90	225.0
47.90	140.0
49.00	841.0
50.00	4311.0
51.00	1266.0
56.10	240.0
57.10	562.0
60.00	267.0
61.00	1274.0
62.00	1324.0
63.00	1391.0
63.90	221.0
64.90	285.0
67.00	109.0
68.00	2557.0
69.00	2322.0
69.90	171.0
72.00	125.0
73.00	1092.0
74.00	4330.0
75.00	12459.0
75.90	1081.0
76.80	147.0
78.90	1345.0
79.90	192.0
80.90	1012.0
81.90	231.0
86.90	820.0
88.00	1052.0
92.00	885.0
92.90	938.0
94.00	2835.0
95.00	24656.0
96.00	1600.0
103.80	135.0
106.00	147.0
116.90	244.0
118.90	195.0
140.90	286.0
142.90	580.0
144.90	344.0
154.80	116.0
170.90	128.0
171.90	429.0
173.00	353.0
173.90	22344.0
174.90	1821.0
176.00	22704.0
176.90	1320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156