

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020124\
 Data File : VU057769.D
 Acq On : 01 Feb 2024 10:23
 Operator : MD/SY
 Sample : VU0201WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0201WBL01

Quant Time: Feb 02 00:33:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Feb 02 00:27:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	41928	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	13603	0.857	ug/l	0.00
Spiked Amount 1.000			Recovery	=	86.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	12619	0.883	ug/l	0.00
Spiked Amount 1.000			Recovery	=	88.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020124\
Data File : VU057769.D
Acq On : 01 Feb 2024 10:23
Operator : MD/SY
Sample : VU0201WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0201WBL01

Quant Time: Feb 02 00:33:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Feb 02 00:27:55 2024
Response via : Initial Calibration




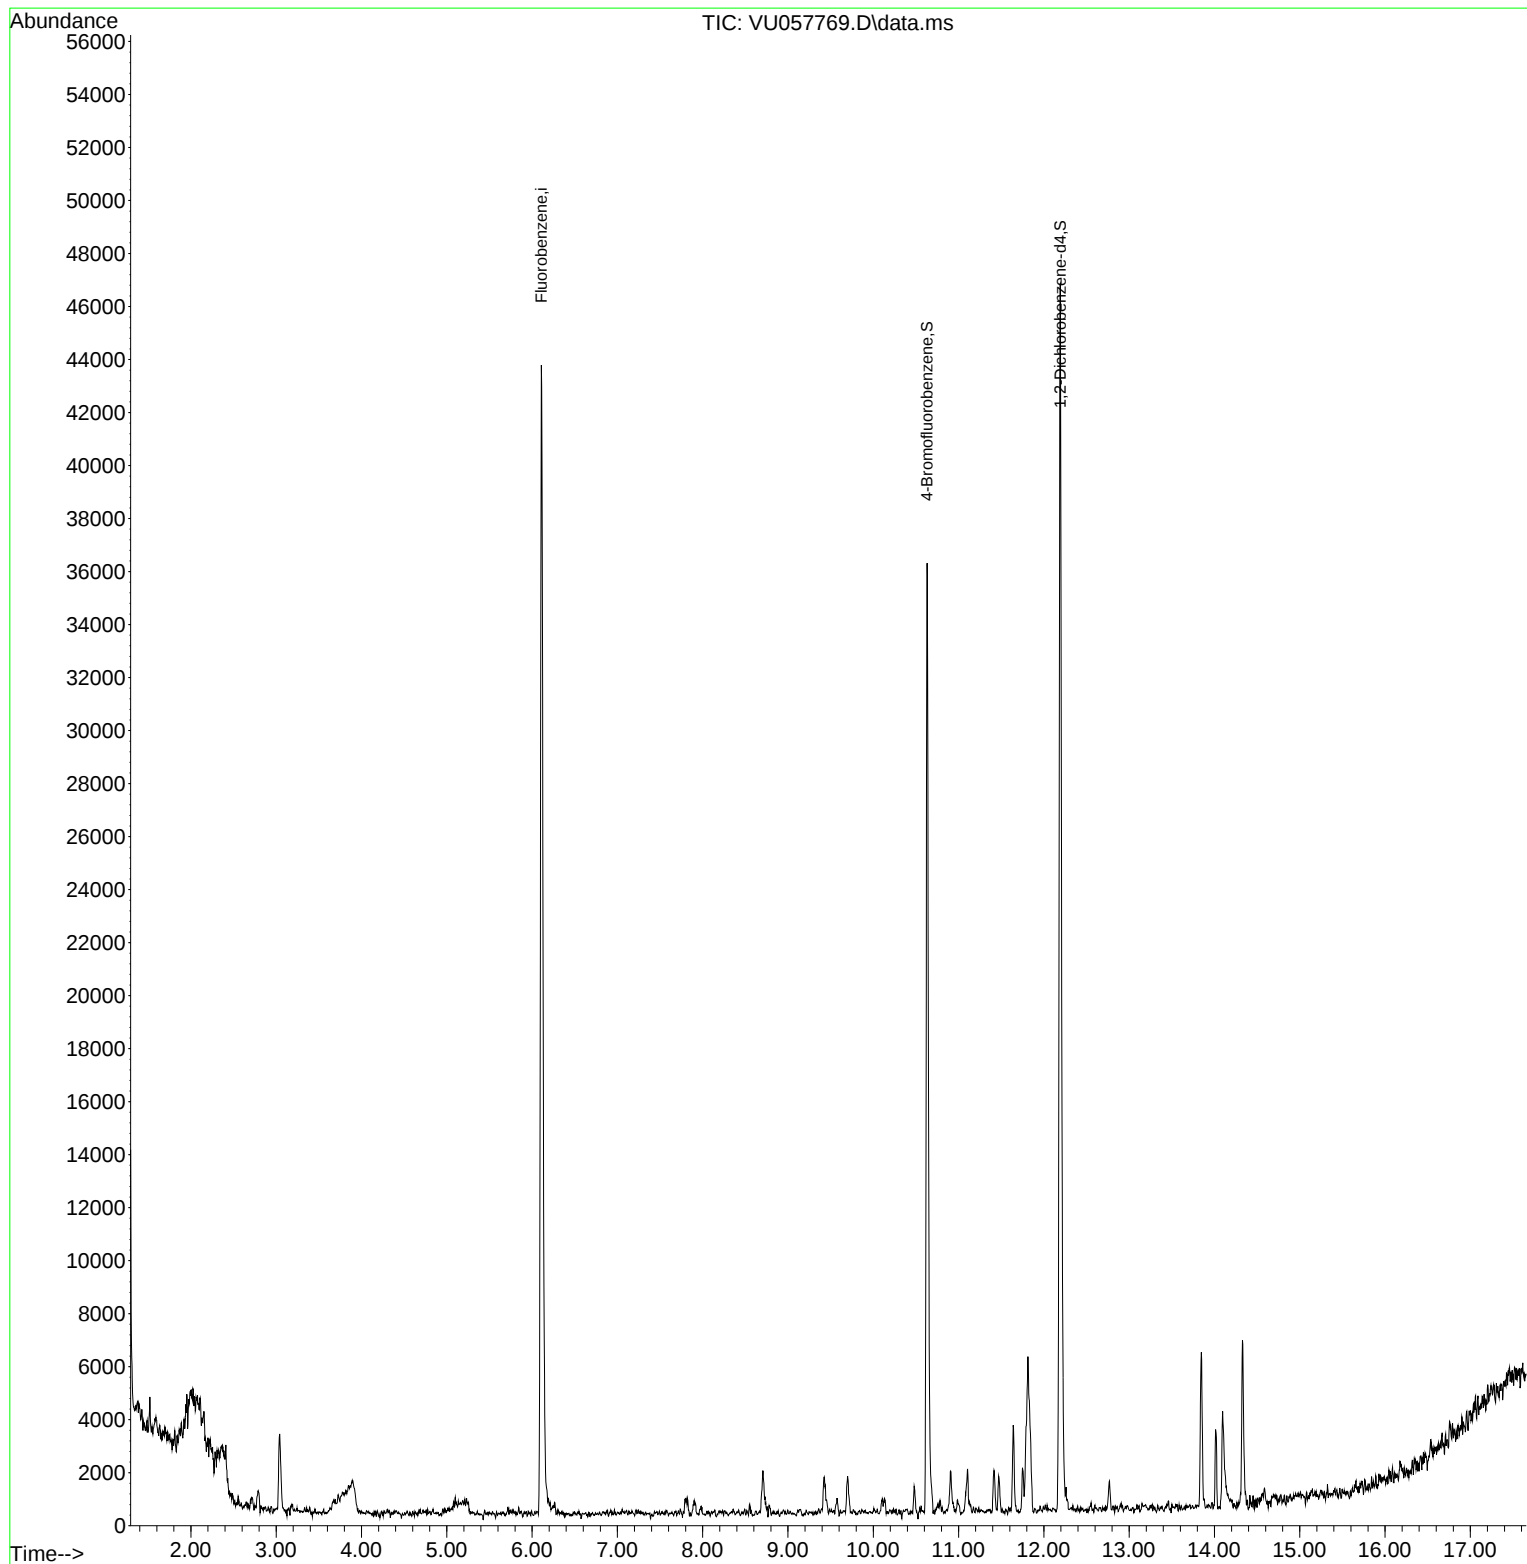


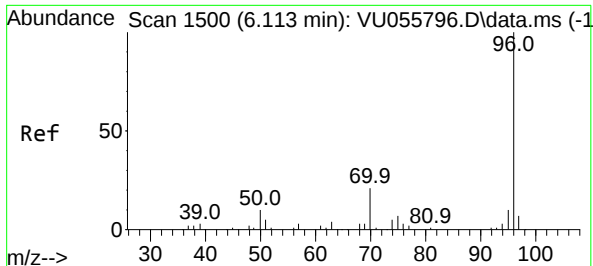

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1499
Delta R.T. -0.003 min
Lab File: VU057769.D
Acq: 01 Feb 2024 10:23




Instrument :
MSVOA_U
ClientSampleId :
VU0201WBL01


Tgt Ion: 96	Resp: 41928
Ion Ratio	Lower Upper
96 100	
70 20.2	16.5 24.7
95 8.7	7.4 11.0
97 6.5	0.0 0.0#

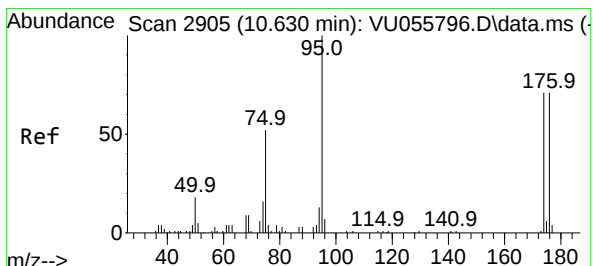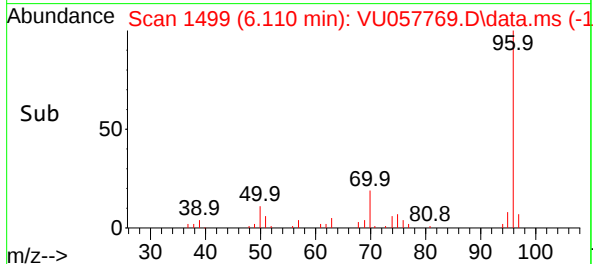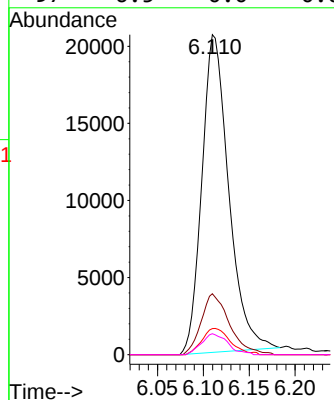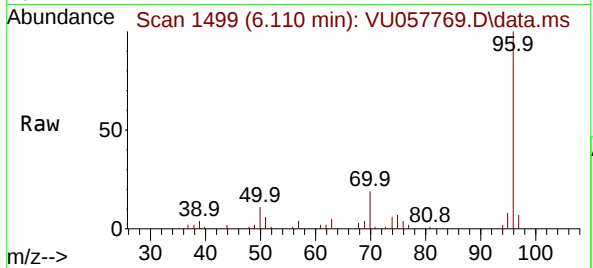

#57
4-Bromofluorobenzene
Concen: 0.857 ug/l
RT: 10.630 min Scan# 2905
Delta R.T. 0.000 min
Lab File: VU057769.D
Acq: 01 Feb 2024 10:23

Tgt Ion: 95	Resp: 13603
Ion Ratio	Lower Upper
95 100	
174 74.7	63.3 94.9
176 73.6	59.3 88.9

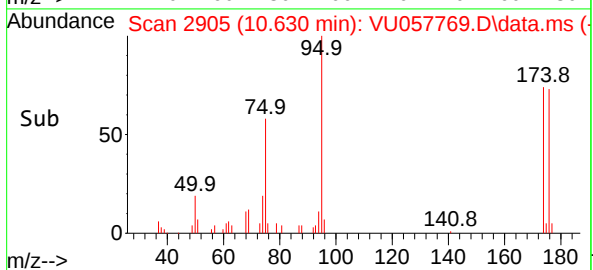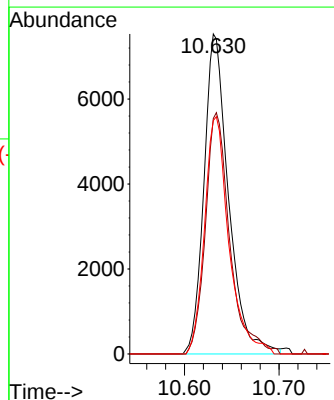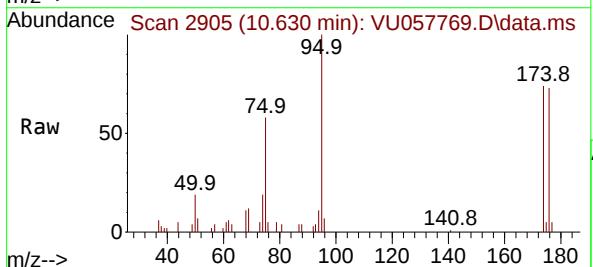

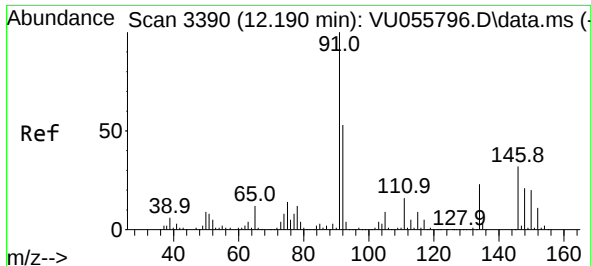

#68

1,2-Dichlorobenzene-d4

Concen: 0.883 ug/l

RT: 12.193 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU057769.D


Acq: 01 Feb 2024 10:23

Instrument :

MSVOA_U

ClientSampleId :

VU0201WBL01

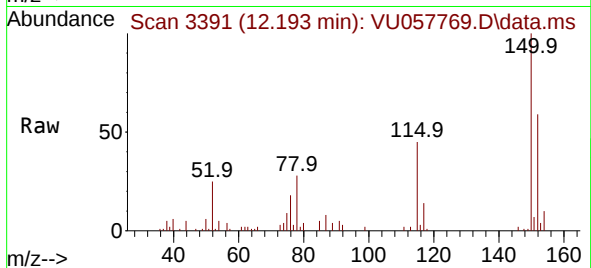

Tgt Ion:152 Resp: 12619

Ion Ratio Lower Upper

152 100

115 70.9 0.0 308.8

150 159.0 0.0 635.0

