


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020124\
Data File : VU057767.D
Acq On : 01 Feb 2024 08:47
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Feb 02 00:27:55 2024

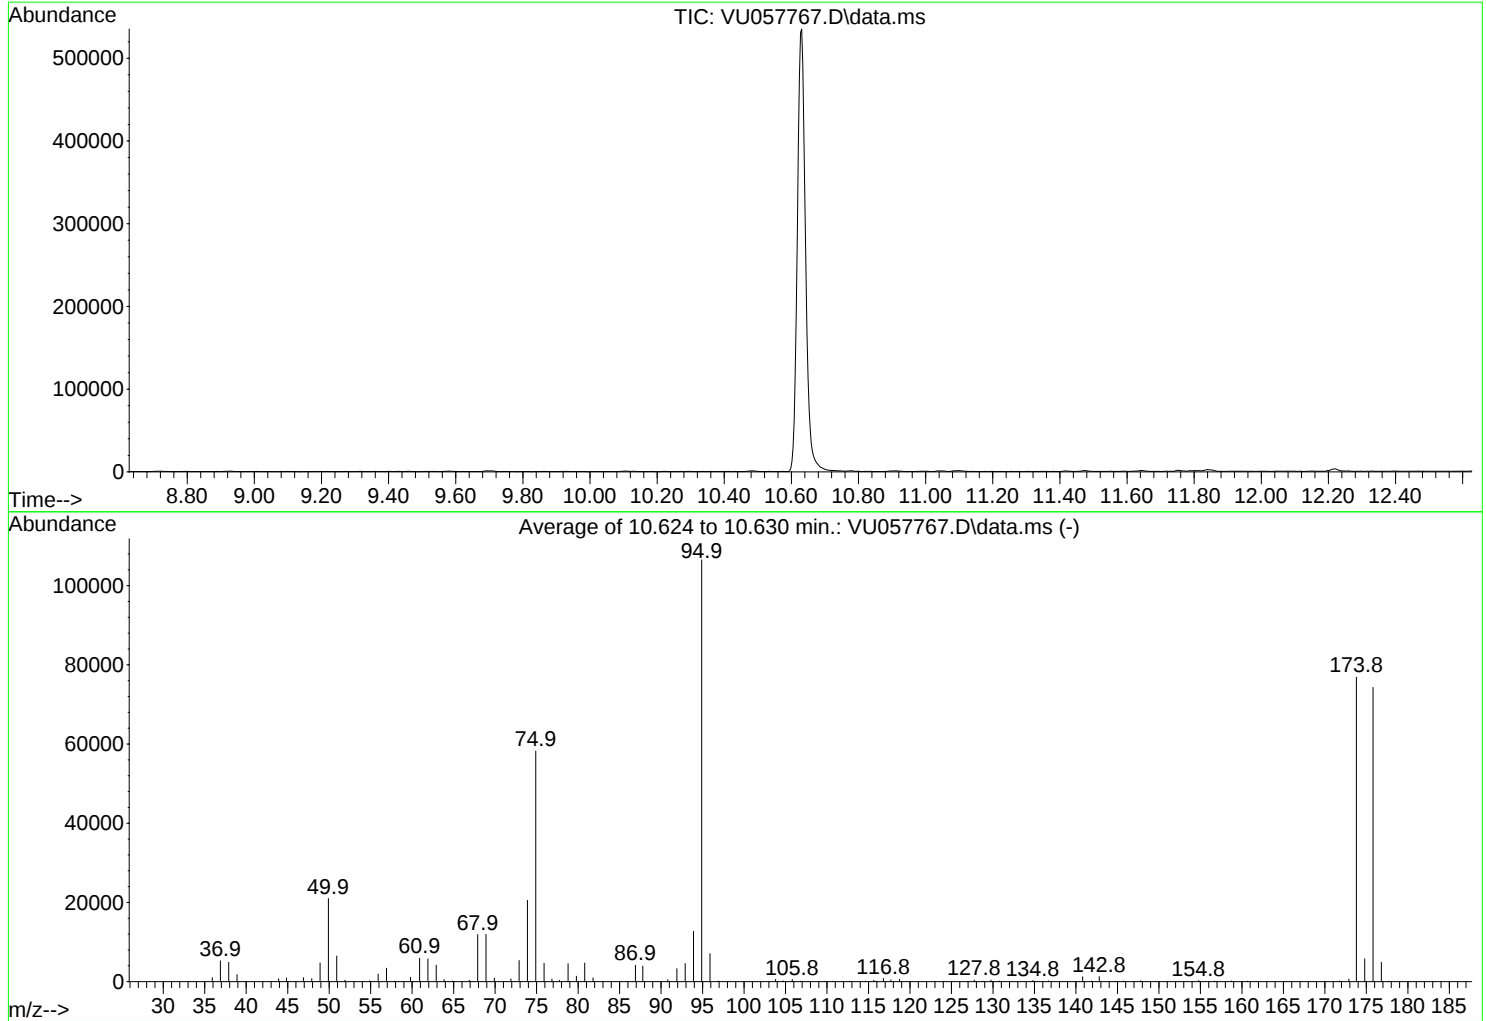

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	20963	PASS
75	95	30	60	54.7	58227	PASS
95	95	100	100	100.0	106528	PASS
96	95	5	9	6.6	7069	PASS
173	174	0.00	2	0.9	666	PASS
174	95	50	100	72.2	76891	PASS
175	174	5	9	7.5	5784	PASS
176	174	95	101	96.6	74307	PASS
177	176	5	9	6.6	4904	PASS