

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052925.D
 Acq On : 02 Feb 2023 15:01
 Operator : JC/MD
 Sample : 01394-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	100	rVB	83352	108735	11.88%	1.656%
2	1.909	169	177	194	rBV	75139	124966	13.65%	1.903%
3	2.334	307	309	312	rBV	236	166	0.02%	0.003%
4	2.555	366	378	395	rVV	177086	287644	31.41%	4.381%
5	2.713	424	427	432	rBV2	480	393	0.04%	0.006%
6	3.041	518	529	541	rBV3	6534	13065	1.43%	0.199%
7	3.182	560	573	588	rBV2	3322	7360	0.80%	0.112%
8	3.301	605	610	613	rBV2	440	372	0.04%	0.006%
9	3.356	623	627	630	rBV2	570	540	0.06%	0.008%
10	3.404	640	642	645	rVB	353	172	0.02%	0.003%
11	3.433	648	651	656	rBV	194	228	0.02%	0.003%
12	3.517	674	677	681	rVB	343	212	0.02%	0.003%
13	3.543	682	685	687	rBV	272	176	0.02%	0.003%
14	3.597	699	702	705	rBB2	235	142	0.02%	0.002%
15	3.684	724	729	732	rBV	227	209	0.02%	0.003%
16	3.800	760	765	767	rBV2	300	267	0.03%	0.004%
17	4.028	831	836	840	rBB2	385	371	0.04%	0.006%
18	4.456	966	969	971	rBV	169	141	0.02%	0.002%
19	4.501	980	983	986	rBB	180	144	0.02%	0.002%
20	4.629	1011	1023	1059	rBV	45338	147791	16.14%	2.251%
21	4.909	1107	1110	1113	rVB2	290	179	0.02%	0.003%
22	4.935	1116	1118	1121	rBV	198	153	0.02%	0.002%
23	5.057	1138	1156	1177	rBV2	169452	379661	41.46%	5.782%
24	5.147	1182	1184	1188	rVB	330	237	0.03%	0.004%
25	5.182	1192	1195	1197	rVB2	321	171	0.02%	0.003%
26	5.263	1216	1220	1222	rBB	274	176	0.02%	0.003%
27	5.285	1222	1227	1236	rBB3	580	849	0.09%	0.013%
28	5.334	1237	1242	1244	rBV	153	186	0.02%	0.003%
29	5.488	1286	1290	1293	rBB	230	206	0.02%	0.003%
30	5.510	1294	1297	1300	rBB2	241	164	0.02%	0.002%
31	5.552	1308	1310	1313	rBV	227	155	0.02%	0.002%
32	5.716	1339	1361	1382	rBV2	335953	915631	100.00%	13.944%
33	5.935	1425	1429	1434	rBB2	268	273	0.03%	0.004%
34	6.067	1468	1470	1475	rVB2	315	221	0.02%	0.003%
35	6.124	1485	1488	1490	rBV	281	160	0.02%	0.002%
36	6.166	1498	1501	1505	rBB	305	241	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052925.D
 Acq On : 02 Feb 2023 15:01
 Operator : JC/MD
 Sample : 01394-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.243	1511	1525	1553	rBV	259378	495970	54.17%	7.553%
38	6.375	1563	1566	1571	rVV2	210	202	0.02%	0.003%
39	6.401	1571	1574	1579	rVB2	338	327	0.04%	0.005%
40	6.430	1580	1583	1586	rBB	169	139	0.02%	0.002%
41	6.469	1591	1595	1597	rBV	269	224	0.02%	0.003%
42	6.497	1602	1604	1606	rBV	267	143	0.02%	0.002%
43	6.539	1606	1617	1630	rBV7	3708	6623	0.72%	0.101%
44	6.684	1648	1662	1680	rBV	211732	411619	44.95%	6.269%
45	6.790	1692	1695	1698	rBV2	347	195	0.02%	0.003%
46	6.809	1698	1701	1704	rVB2	537	314	0.03%	0.005%
47	6.919	1732	1735	1740	rBV	221	260	0.03%	0.004%
48	7.038	1768	1772	1775	rBV	188	168	0.02%	0.003%
49	7.192	1812	1820	1822	rBV4	1716	2231	0.24%	0.034%
50	7.562	1923	1935	1950	rBV	106106	186849	20.41%	2.846%
51	7.697	1970	1977	1981	rBV4	858	1067	0.12%	0.016%
52	7.803	2003	2010	2012	rBV3	1146	1297	0.14%	0.020%
53	7.893	2025	2038	2054	rBV	394451	682199	74.51%	10.389%
54	8.128	2108	2111	2114	rBB2	362	185	0.02%	0.003%
55	8.176	2115	2126	2144	rBV	74902	131707	14.38%	2.006%
56	8.259	2149	2152	2155	rBV2	403	297	0.03%	0.005%
57	8.388	2188	2192	2195	rBV2	296	247	0.03%	0.004%
58	8.542	2237	2240	2241	rBV	631	364	0.04%	0.006%
59	8.578	2249	2251	2254	rVB	257	147	0.02%	0.002%
60	8.652	2260	2274	2300	rBV2	150805	341007	37.24%	5.193%
61	8.793	2315	2318	2324	rVB2	332	204	0.02%	0.003%
62	8.973	2371	2374	2376	rBV	224	184	0.02%	0.003%
63	9.047	2391	2397	2400	rBV	233	327	0.04%	0.005%
64	9.275	2465	2468	2472	rVB2	295	216	0.02%	0.003%
65	9.298	2473	2475	2478	rBV	320	206	0.02%	0.003%
66	9.414	2499	2511	2535	rBV	351721	605224	66.10%	9.217%
67	9.523	2543	2545	2547	rVB	376	152	0.02%	0.002%
68	9.565	2551	2558	2561	rBV3	1210	1428	0.16%	0.022%
69	9.603	2568	2570	2576	rVB2	351	308	0.03%	0.005%
70	9.690	2588	2597	2606	rVB4	2812	4306	0.47%	0.066%
71	9.793	2626	2629	2631	rBV2	267	175	0.02%	0.003%
72	9.809	2632	2634	2640	rVB	402	335	0.04%	0.005%
73	9.848	2641	2646	2649	rBV	264	246	0.03%	0.004%
74	10.021	2695	2700	2701	rBV	177	158	0.02%	0.002%
75	10.034	2701	2704	2710	rVB	283	228	0.02%	0.003%
76	10.115	2715	2729	2730	rBV4	2480	3621	0.40%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052925.D
 Acq On : 02 Feb 2023 15:01
 Operator : JC/MD
 Sample : 01394-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.221	2757	2762	2765	rBV	200	232	0.03%	0.004%
78	10.250	2767	2771	2775	rVB3	447	388	0.04%	0.006%
79	10.481	2833	2843	2856	rBB3	1839	2834	0.31%	0.043%
80	10.529	2856	2858	2862	rBV	271	233	0.03%	0.004%
81	10.639	2890	2892	2895	rBV	202	158	0.02%	0.002%
82	10.706	2909	2913	2917	rBV2	243	245	0.03%	0.004%
83	10.758	2917	2929	2949	rBV	284631	455401	49.74%	6.935%
84	11.404	3127	3130	3132	rBV	182	144	0.02%	0.002%
85	11.468	3147	3150	3155	rBV	247	278	0.03%	0.004%
86	11.613	3192	3195	3196	rBV	247	167	0.02%	0.003%
87	11.742	3232	3235	3240	rVB2	454	423	0.05%	0.006%
88	11.809	3244	3256	3274	rBV	354455	561147	61.29%	8.546%
89	12.192	3361	3375	3401	rBV	377290	624886	68.25%	9.516%
90	12.764	3549	3553	3558	rVB2	781	776	0.08%	0.012%
91	13.124	3662	3665	3670	rBV	224	177	0.02%	0.003%
92	13.147	3670	3672	3676	rVB2	355	186	0.02%	0.003%
93	13.221	3685	3695	3706	rBV4	7532	11868	1.30%	0.181%
94	13.841	3878	3888	3895	rBV6	4227	6470	0.71%	0.099%
95	14.082	3960	3963	3966	rBV2	667	599	0.07%	0.009%
96	14.295	4026	4029	4030	rBV	352	203	0.02%	0.003%
97	14.327	4030	4039	4053	rVB2	16528	25777	2.82%	0.393%
98	14.420	4066	4068	4073	rBV2	216	223	0.02%	0.003%
99	14.510	4091	4096	4101	rBV3	325	389	0.04%	0.006%
100	14.690	4149	4152	4154	rVB2	585	320	0.03%	0.005%


Sum of corrected areas: 6566380

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052925.D
Acq On : 02 Feb 2023 15:01
Operator : JC/MD
Sample : 01394-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

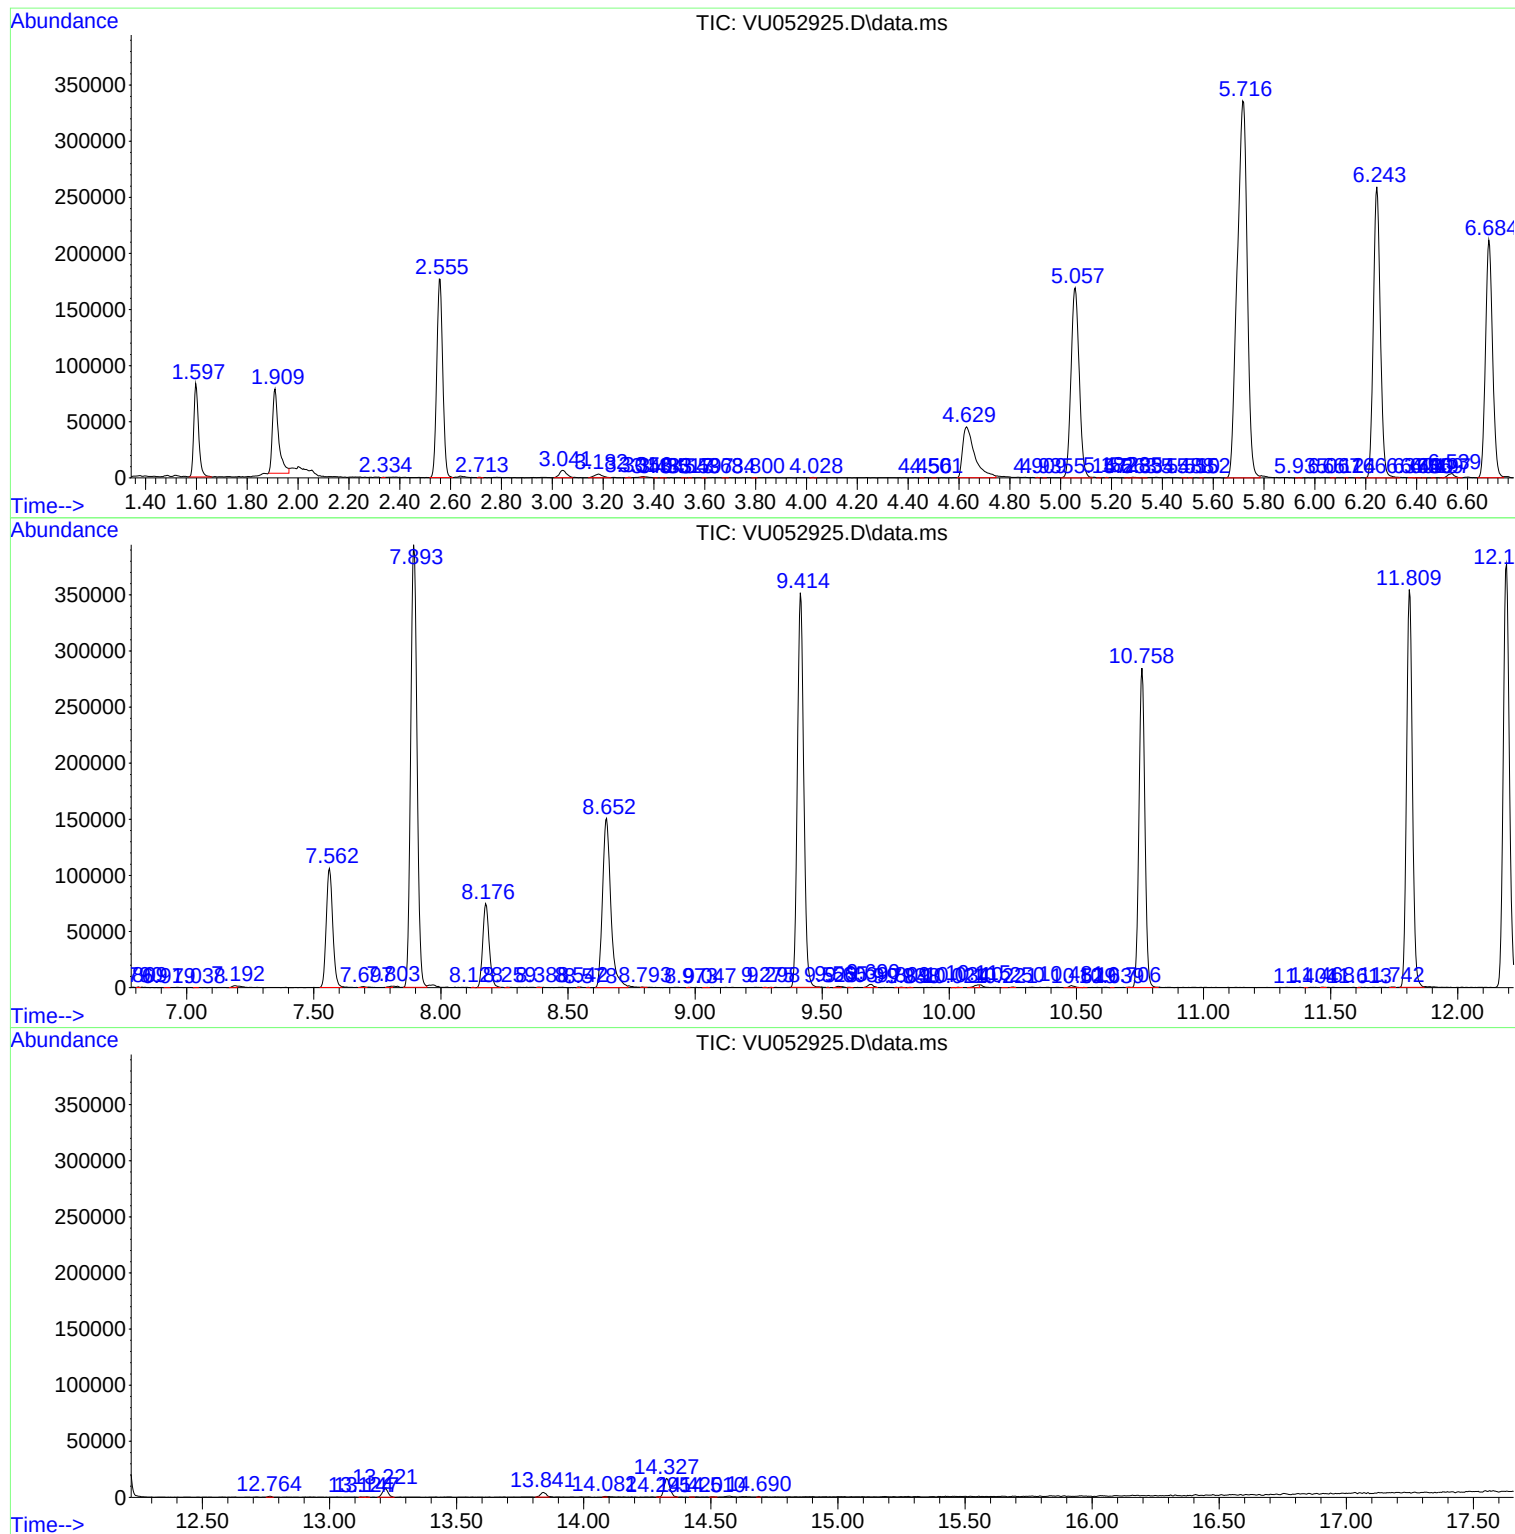

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052925.D
Acq On : 02 Feb 2023 15:01
Operator : JC/MD
Sample : 01394-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052925.D
Acq On : 02 Feb 2023 15:01
Operator : JC/MD
Sample : 01394-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------