

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052927.D
 Acq On : 02 Feb 2023 15:48
 Operator : JC/MD
 Sample : 01381-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	99	rVB	91990	119330	12.70%	1.693%
2	1.906	169	176	195	rBV	81781	126939	13.51%	1.801%
3	2.559	367	379	395	rBV	194239	316616	33.70%	4.492%
4	2.713	425	427	429	rVV2	340	172	0.02%	0.002%
5	2.874	474	477	481	rBV	167	144	0.02%	0.002%
6	3.041	519	529	541	rBV3	3462	6630	0.71%	0.094%
7	3.285	601	605	607	rBV	215	165	0.02%	0.002%
8	3.327	615	618	621	rBV	191	181	0.02%	0.003%
9	3.366	627	630	632	rBV	245	173	0.02%	0.002%
10	3.485	664	667	670	rBV	220	182	0.02%	0.003%
11	3.562	688	691	696	rBB	144	149	0.02%	0.002%
12	3.594	697	701	704	rBB2	251	194	0.02%	0.003%
13	3.645	714	717	719	rVB	251	143	0.02%	0.002%
14	3.687	727	730	732	rBB	250	150	0.02%	0.002%
15	3.764	750	754	757	rBV2	284	278	0.03%	0.004%
16	3.957	812	814	819	rVB2	291	240	0.03%	0.003%
17	4.009	828	830	836	rVB2	229	203	0.02%	0.003%
18	4.092	854	856	860	rVB	279	170	0.02%	0.002%
19	4.153	870	875	878	rBV	197	227	0.02%	0.003%
20	4.250	900	905	906	rBV	199	172	0.02%	0.002%
21	4.378	940	945	948	rBV	172	206	0.02%	0.003%
22	4.507	981	985	988	rBV	183	221	0.02%	0.003%
23	4.626	1010	1022	1047	rBV	49839	147235	15.67%	2.089%
24	4.909	1108	1110	1115	rVB	378	257	0.03%	0.004%
25	4.944	1116	1121	1126	rBV2	326	437	0.05%	0.006%
26	5.057	1138	1156	1180	rBV	178315	391891	41.71%	5.560%
27	5.452	1273	1279	1282	rBV	149	196	0.02%	0.003%
28	5.520	1295	1300	1303	rBB	153	183	0.02%	0.003%
29	5.591	1317	1322	1327	rBB	205	273	0.03%	0.004%
30	5.719	1340	1362	1385	rBV2	348867	939458	100.00%	13.328%
31	6.050	1462	1465	1467	rBV2	269	168	0.02%	0.002%
32	6.108	1478	1483	1485	rBV2	323	245	0.03%	0.003%
33	6.121	1485	1487	1490	rVB2	344	170	0.02%	0.002%
34	6.243	1509	1525	1545	rBV	281701	530807	56.50%	7.531%
35	6.404	1573	1575	1578	rBB2	272	147	0.02%	0.002%
36	6.443	1584	1587	1589	rBB	285	161	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052927.D
 Acq On : 02 Feb 2023 15:48
 Operator : JC/MD
 Sample : 01381-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.475	1593	1597	1600	rBV2	359	319	0.03%	0.005%
38	6.536	1607	1616	1629	rVB7	9541	17670	1.88%	0.251%
39	6.607	1633	1638	1639	rBV2	230	174	0.02%	0.002%
40	6.684	1649	1662	1680	rBV	215108	418687	44.57%	5.940%
41	6.793	1690	1696	1697	rBV	443	315	0.03%	0.004%
42	6.951	1742	1745	1747	rBV	202	148	0.02%	0.002%
43	7.092	1785	1789	1792	rBB	154	159	0.02%	0.002%
44	7.150	1804	1807	1810	rBV2	300	240	0.03%	0.003%
45	7.195	1810	1821	1827	rBV7	1541	3169	0.34%	0.045%
46	7.311	1854	1857	1861	rVV2	198	169	0.02%	0.002%
47	7.410	1885	1888	1890	rBV	284	203	0.02%	0.003%
48	7.520	1918	1922	1923	rBV	202	167	0.02%	0.002%
49	7.562	1923	1935	1952	rBV	112420	197900	21.07%	2.808%
50	7.648	1960	1962	1965	rVB	305	168	0.02%	0.002%
51	7.690	1970	1975	1978	rBV3	849	835	0.09%	0.012%
52	7.832	2016	2019	2024	rBV	240	258	0.03%	0.004%
53	7.893	2024	2038	2057	rBV	430978	733855	78.11%	10.411%
54	8.092	2096	2100	2104	rVB2	232	246	0.03%	0.003%
55	8.176	2114	2126	2146	rBV	78343	136412	14.52%	1.935%
56	8.269	2152	2155	2159	rVB	280	188	0.02%	0.003%
57	8.288	2159	2161	2164	rVB2	299	210	0.02%	0.003%
58	8.311	2165	2168	2170	rBV	330	250	0.03%	0.004%
59	8.452	2208	2212	2213	rBV	319	240	0.03%	0.003%
60	8.468	2213	2217	2219	rBV2	1156	857	0.09%	0.012%
61	8.529	2231	2236	2239	rBV	270	228	0.02%	0.003%
62	8.587	2250	2254	2256	rBV	199	177	0.02%	0.003%
63	8.648	2258	2273	2306	rBV2	158096	342301	36.44%	4.856%
64	8.896	2347	2350	2355	rBV2	376	322	0.03%	0.005%
65	9.012	2384	2386	2389	rBB2	280	152	0.02%	0.002%
66	9.041	2393	2395	2396	rBV	283	157	0.02%	0.002%
67	9.282	2465	2470	2473	rBV	249	309	0.03%	0.004%
68	9.414	2497	2511	2531	rBV	383544	662635	70.53%	9.401%
69	9.687	2591	2596	2603	rBV2	610	910	0.10%	0.013%
70	9.748	2612	2615	2622	rBB	347	422	0.04%	0.006%
71	9.861	2645	2650	2654	rBB	252	276	0.03%	0.004%
72	9.889	2655	2659	2662	rBV	185	211	0.02%	0.003%
73	9.906	2662	2664	2666	rVB	327	167	0.02%	0.002%
74	9.928	2666	2671	2673	rBV	215	239	0.03%	0.003%
75	10.201	2753	2756	2758	rBV	223	162	0.02%	0.002%
76	10.381	2809	2812	2814	rBV	269	202	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052927.D
 Acq On : 02 Feb 2023 15:48
 Operator : JC/MD
 Sample : 01381-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.491	2841	2846	2851	rVB2	431	439	0.05%	0.006%
78	10.758	2915	2929	2943	rVV	283653	457059	48.65%	6.484%
79	10.886	2964	2969	2978	rVB4	1318	1995	0.21%	0.028%
80	10.928	2980	2982	2990	rVB	280	218	0.02%	0.003%
81	11.320	3101	3104	3106	rBV	273	186	0.02%	0.003%
82	11.356	3112	3115	3120	rVB	316	304	0.03%	0.004%
83	11.381	3120	3123	3127	rBV	225	238	0.03%	0.003%
84	11.446	3140	3143	3146	rBV	204	195	0.02%	0.003%
85	11.465	3146	3149	3154	rVB2	361	322	0.03%	0.005%
86	11.748	3228	3237	3243	rBV4	2829	4092	0.44%	0.058%
87	11.809	3243	3256	3276	rBV	397349	638452	67.96%	9.058%
88	12.063	3328	3335	3344	rBV5	1915	3038	0.32%	0.043%
89	12.192	3362	3375	3395	rBV2	436658	777123	82.72%	11.025%
90	12.352	3421	3425	3426	rBV2	304	187	0.02%	0.003%
91	12.430	3445	3449	3452	rBV	229	250	0.03%	0.004%
92	12.767	3546	3554	3557	rBV3	945	1244	0.13%	0.018%
93	13.221	3687	3695	3704	rVB5	2420	3735	0.40%	0.053%
94	13.410	3749	3754	3758	rVB2	367	312	0.03%	0.004%
95	13.635	3821	3824	3834	rVB	450	435	0.05%	0.006%
96	13.684	3835	3839	3842	rBV2	300	273	0.03%	0.004%
97	13.838	3877	3887	3904	rVB2	27087	42495	4.52%	0.603%
98	14.330	4032	4040	4050	rVB3	5833	9350	1.00%	0.133%
99	14.372	4050	4053	4056	rBV2	349	249	0.03%	0.004%
100	14.455	4076	4079	4084	rVB2	391	312	0.03%	0.004%




Sum of corrected areas: 7048725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052927.D
Acq On : 02 Feb 2023 15:48
Operator : JC/MD
Sample : 01381-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

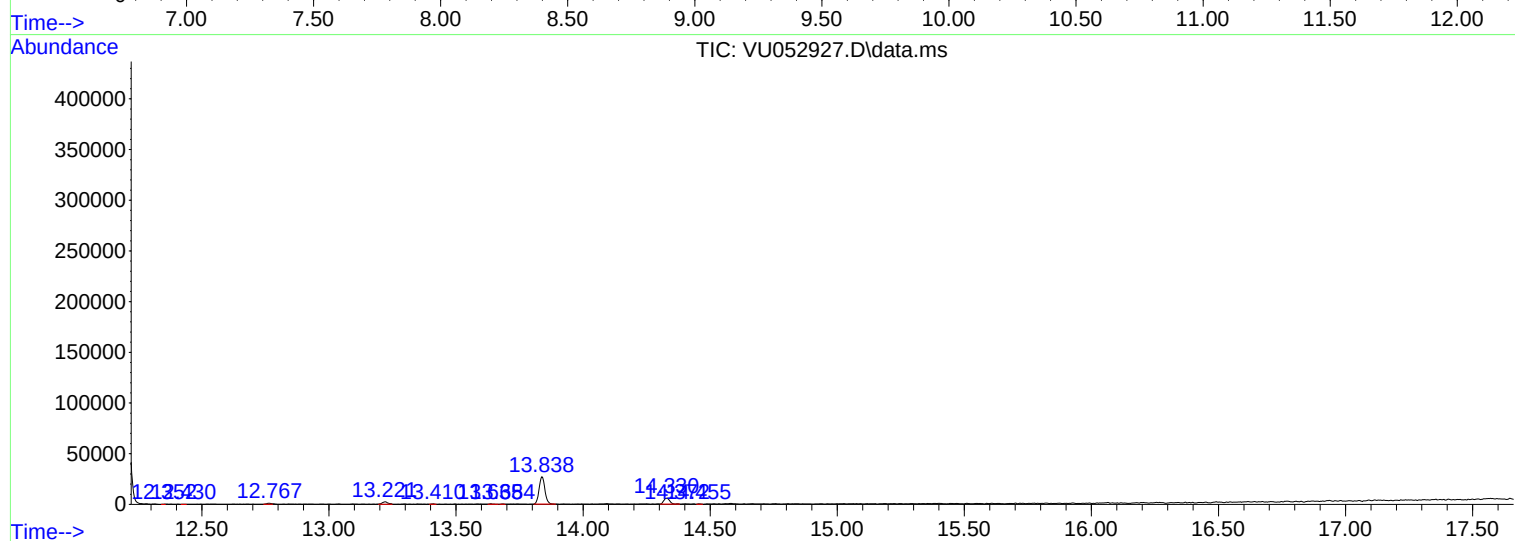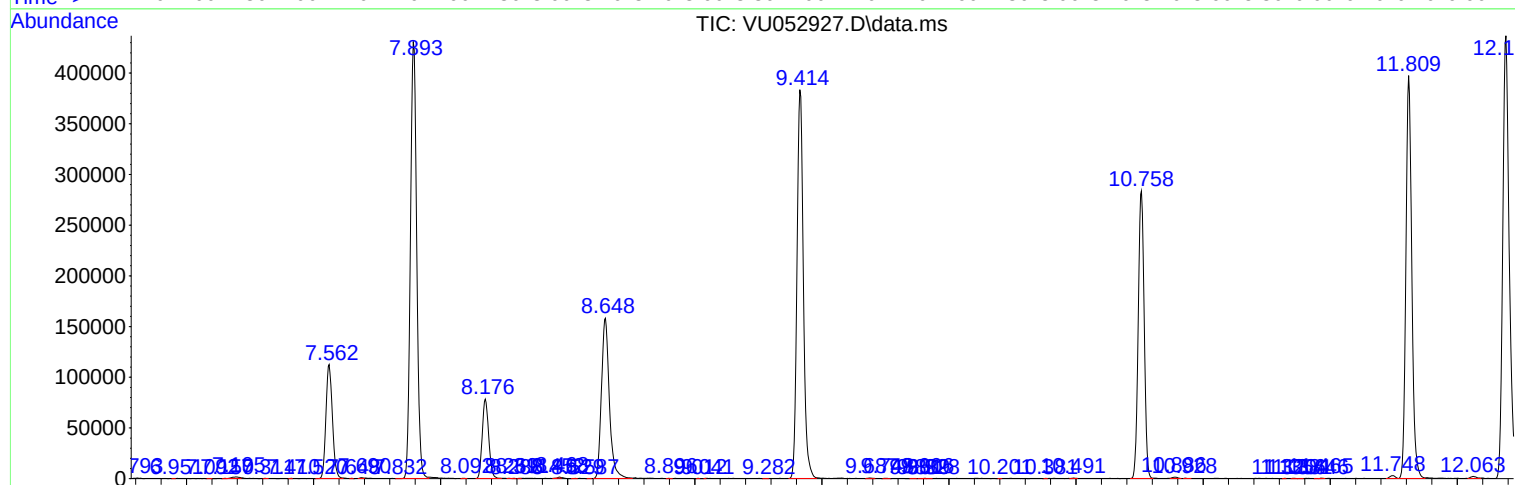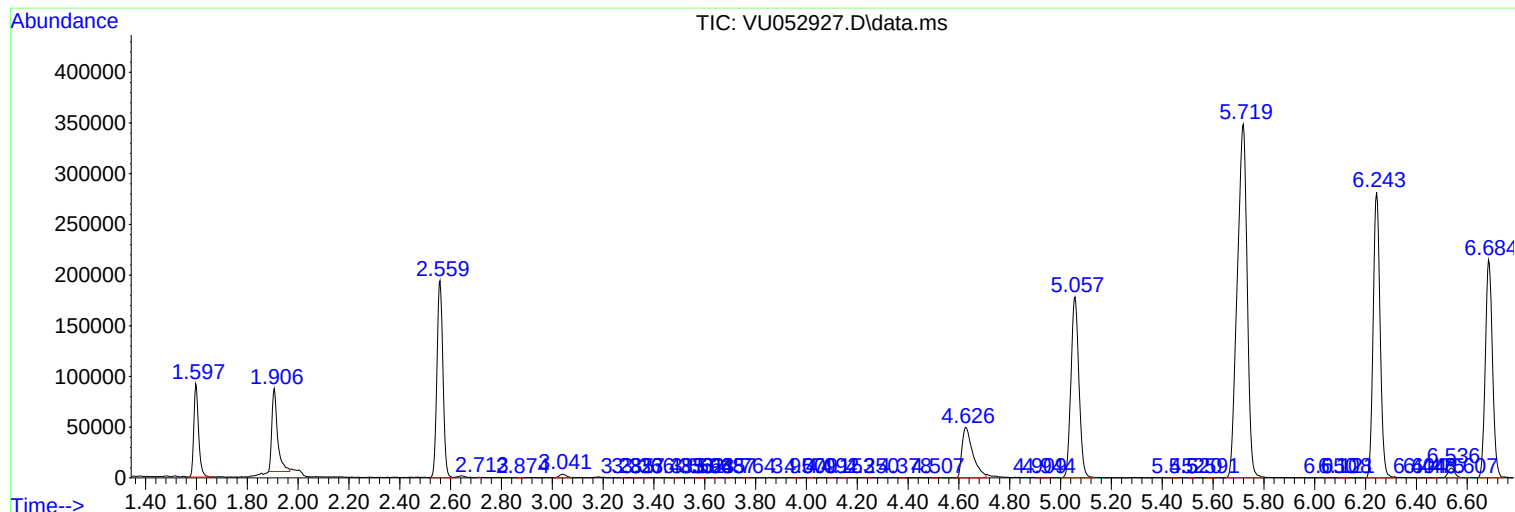

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052927.D
Acq On : 02 Feb 2023 15:48
Operator : JC/MD
Sample : 01381-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052927.D
Acq On : 02 Feb 2023 15:48
Operator : JC/MD
Sample : 01381-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc