

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052931.D
 Acq On : 02 Feb 2023 17:22
 Operator : JC/MD
 Sample : 01381-17DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44Q5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	84110	108552	6.65%	1.256%
2	1.906	169	176	192	rBV	75444	111713	6.84%	1.292%
3	2.488	352	357	361	rVB2	307	333	0.02%	0.004%
4	2.559	366	379	395	rVV	187121	301836	18.48%	3.492%
5	2.710	421	426	432	rVB2	454	501	0.03%	0.006%
6	2.764	437	443	446	rBV2	368	458	0.03%	0.005%
7	2.932	492	495	498	rBV	169	160	0.01%	0.002%
8	3.038	516	528	547	rVB2	10960	22226	1.36%	0.257%
9	3.182	560	573	588	rBV2	2518	6377	0.39%	0.074%
10	3.282	600	604	605	rBV	261	197	0.01%	0.002%
11	3.430	645	650	652	rBV	268	196	0.01%	0.002%
12	3.443	652	654	657	rVB	190	146	0.01%	0.002%
13	3.510	671	675	678	rBB	170	167	0.01%	0.002%
14	3.645	713	717	720	rBV	337	271	0.02%	0.003%
15	3.713	735	738	742	rVB2	397	291	0.02%	0.003%
16	3.816	767	770	773	rBV	242	218	0.01%	0.003%
17	3.973	816	819	823	rBB	179	159	0.01%	0.002%
18	4.041	837	840	844	rBB	207	171	0.01%	0.002%
19	4.079	848	852	855	rBV	166	172	0.01%	0.002%
20	4.160	875	877	880	rBV2	234	161	0.01%	0.002%
21	4.211	889	893	896	rBB	167	164	0.01%	0.002%
22	4.285	913	916	919	rBB	179	139	0.01%	0.002%
23	4.504	982	984	989	rVB	374	230	0.01%	0.003%
24	4.629	1006	1023	1027	rBV	52606	105111	6.43%	1.216%
25	4.922	1110	1114	1117	rVV2	340	260	0.02%	0.003%
26	4.941	1117	1120	1123	rVB2	339	281	0.02%	0.003%
27	5.057	1139	1156	1181	rBV	170069	374728	22.94%	4.335%
28	5.211	1200	1204	1206	rVV	224	170	0.01%	0.002%
29	5.275	1222	1224	1226	rBV	277	183	0.01%	0.002%
30	5.369	1247	1253	1256	rBV2	402	460	0.03%	0.005%
31	5.427	1267	1271	1274	rBB2	292	278	0.02%	0.003%
32	5.488	1283	1290	1291	rBV	191	236	0.01%	0.003%
33	5.610	1324	1328	1331	rBB	192	175	0.01%	0.002%
34	5.719	1341	1362	1386	rBV2	330300	893575	54.70%	10.337%
35	5.902	1415	1419	1422	rVB3	275	203	0.01%	0.002%
36	5.954	1431	1435	1438	rBB2	297	229	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052931.D
 Acq On : 02 Feb 2023 17:22
 Operator : JC/MD
 Sample : 01381-17DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44Q5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.005	1447	1451	1453	rBB2	236	183	0.01%	0.002%
38	6.060	1465	1468	1472	rVB	185	141	0.01%	0.002%
39	6.124	1484	1488	1491	rBV2	383	284	0.02%	0.003%
40	6.243	1510	1525	1552	rBV	279894	530908	32.50%	6.142%
41	6.439	1583	1586	1590	rBB	256	204	0.01%	0.002%
42	6.462	1591	1593	1598	rBV	357	285	0.02%	0.003%
43	6.536	1602	1616	1643	rBV	394817	733155	44.88%	8.481%
44	6.684	1646	1662	1682	rBV	208971	403573	24.70%	4.669%
45	6.796	1692	1697	1698	rBV	404	268	0.02%	0.003%
46	6.964	1744	1749	1751	rBB	181	174	0.01%	0.002%
47	6.992	1756	1758	1764	rBB	176	198	0.01%	0.002%
48	7.044	1770	1774	1778	rBV2	281	301	0.02%	0.003%
49	7.185	1810	1818	1820	rBV4	1716	1824	0.11%	0.021%
50	7.301	1850	1854	1857	rBV	171	199	0.01%	0.002%
51	7.562	1921	1935	1950	rBV	108520	189979	11.63%	2.198%
52	7.812	2011	2013	2016	rBB	240	142	0.01%	0.002%
53	7.893	2025	2038	2058	rBV	412326	698401	42.75%	8.079%
54	8.031	2078	2081	2085	rVB3	577	399	0.02%	0.005%
55	8.176	2115	2126	2144	rVV	75854	130040	7.96%	1.504%
56	8.359	2179	2183	2188	rBV	265	256	0.02%	0.003%
57	8.385	2188	2191	2193	rBV	200	144	0.01%	0.002%
58	8.433	2203	2206	2209	rBV2	323	253	0.02%	0.003%
59	8.471	2209	2218	2220	rBV2	644	775	0.05%	0.009%
60	8.578	2247	2251	2254	rBV	200	215	0.01%	0.002%
61	8.645	2259	2272	2304	rVV2	152709	329722	20.18%	3.814%
62	8.841	2330	2333	2341	rVB	518	479	0.03%	0.006%
63	8.880	2342	2345	2346	rBV	306	159	0.01%	0.002%
64	8.976	2372	2375	2381	rVB2	221	175	0.01%	0.002%
65	9.108	2412	2416	2422	rBB	279	228	0.01%	0.003%
66	9.169	2433	2435	2441	rBB	206	213	0.01%	0.002%
67	9.198	2441	2444	2447	rBB	199	160	0.01%	0.002%
68	9.279	2466	2469	2475	rBB	164	191	0.01%	0.002%
69	9.330	2482	2485	2487	rBV	210	170	0.01%	0.002%
70	9.414	2497	2511	2517	rBV	399210	693895	42.48%	8.027%
71	9.697	2593	2599	2603	rBV2	498	568	0.03%	0.007%
72	9.751	2612	2616	2618	rBV	189	187	0.01%	0.002%
73	9.848	2643	2646	2649	rVV	245	180	0.01%	0.002%
74	9.931	2668	2672	2675	rBV	234	239	0.01%	0.003%
75	10.047	2705	2708	2711	rBV	219	188	0.01%	0.002%
76	10.272	2776	2778	2782	rBV	296	221	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
 Data File : VU052931.D
 Acq On : 02 Feb 2023 17:22
 Operator : JC/MD
 Sample : 01381-17DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44Q5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.401	2815	2818	2822	rBV	172	192	0.01%	0.002%
78	10.455	2829	2835	2837	rBV2	313	279	0.02%	0.003%
79	10.484	2841	2844	2846	rVV	244	153	0.01%	0.002%
80	10.510	2849	2852	2855	rVV2	213	141	0.01%	0.002%
81	10.671	2898	2902	2909	rVB	276	431	0.03%	0.005%
82	10.709	2910	2914	2916	rBV	177	188	0.01%	0.002%
83	10.758	2916	2929	2943	rBV	280499	445192	27.25%	5.150%
84	10.889	2964	2970	2975	rBV	545	648	0.04%	0.007%
85	11.613	3192	3195	3198	rBV	329	263	0.02%	0.003%
86	11.648	3203	3206	3210	rVB	298	208	0.01%	0.002%
87	11.745	3226	3236	3245	rBV2	18478	28133	1.72%	0.325%
88	11.809	3245	3256	3277	rVV2	408694	813944	49.83%	9.416%
89	11.976	3306	3308	3313	rBV2	301	206	0.01%	0.002%
90	12.204	3361	3379	3404	rBV2	723536	1633579	100.00%	18.898%
91	12.764	3547	3553	3554	rBV	598	442	0.03%	0.005%
92	12.963	3612	3615	3617	rBV2	245	164	0.01%	0.002%
93	13.208	3683	3691	3694	rBV4	4107	5094	0.31%	0.059%
94	13.349	3732	3735	3739	rBV	248	212	0.01%	0.002%
95	13.372	3739	3742	3746	rVB	344	206	0.01%	0.002%
96	13.394	3746	3749	3754	rBV	335	313	0.02%	0.004%
97	13.655	3827	3830	3834	rBV2	263	203	0.01%	0.002%
98	13.838	3876	3887	3904	rVB2	36327	57447	3.52%	0.665%
99	14.330	4031	4040	4049	rBV5	4264	6272	0.38%	0.073%
100	14.761	4171	4174	4179	rBV2	443	444	0.03%	0.005%


Sum of corrected areas: 8644357

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052931.D
Acq On : 02 Feb 2023 17:22
Operator : JC/MD
Sample : 01381-17DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44Q5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

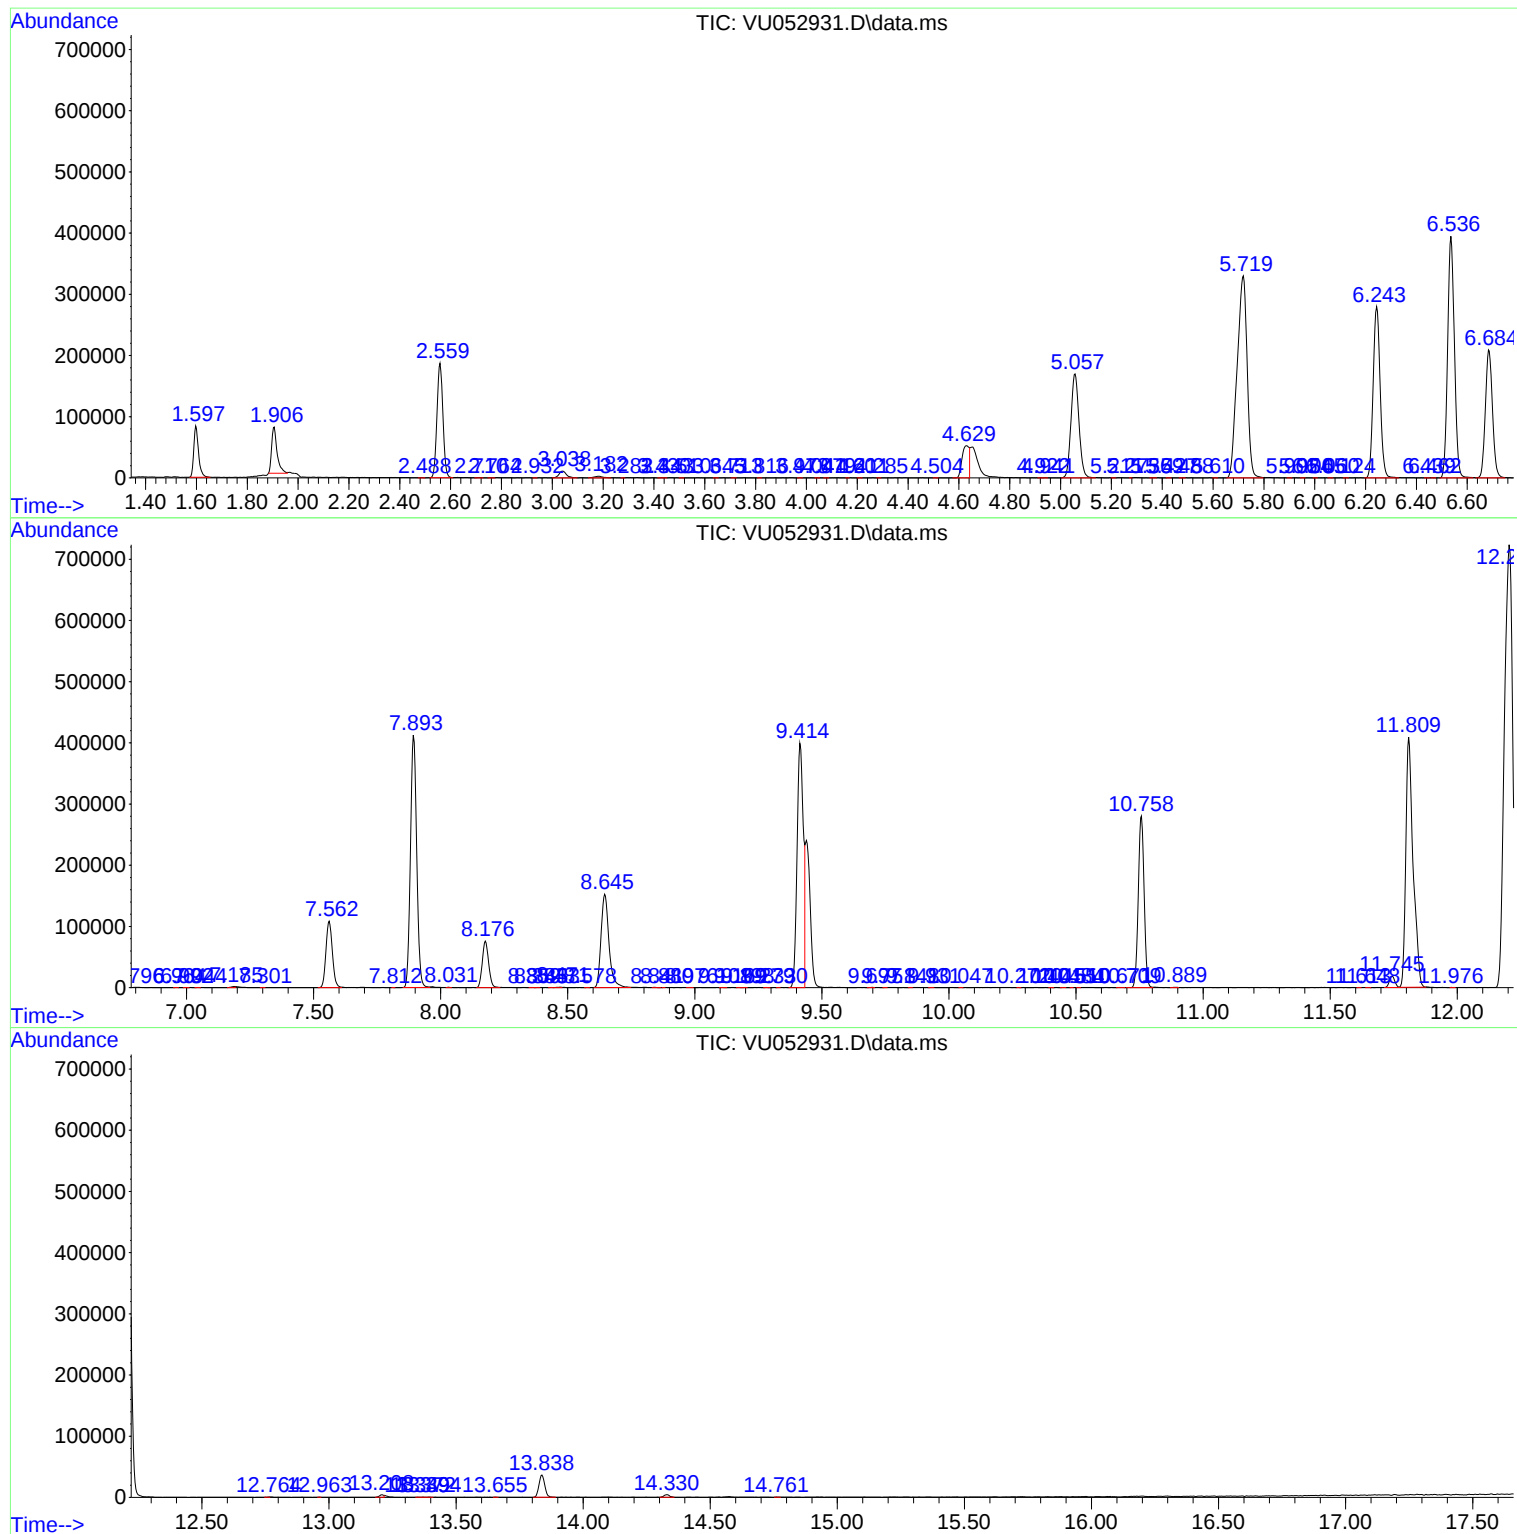

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052931.D
Acq On : 02 Feb 2023 17:22
Operator : JC/MD
Sample : 01381-17DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44Q5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052931.D
Acq On : 02 Feb 2023 17:22
Operator : JC/MD
Sample : 01381-17DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44Q5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------