


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020223\
Data File : VU052919.D
Acq On : 02 Feb 2023 11:32
Operator : JC/MD
Sample : BFB157
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB157

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Title : VOC Analysis
Last Update : Fri Feb 03 23:44:08 2023

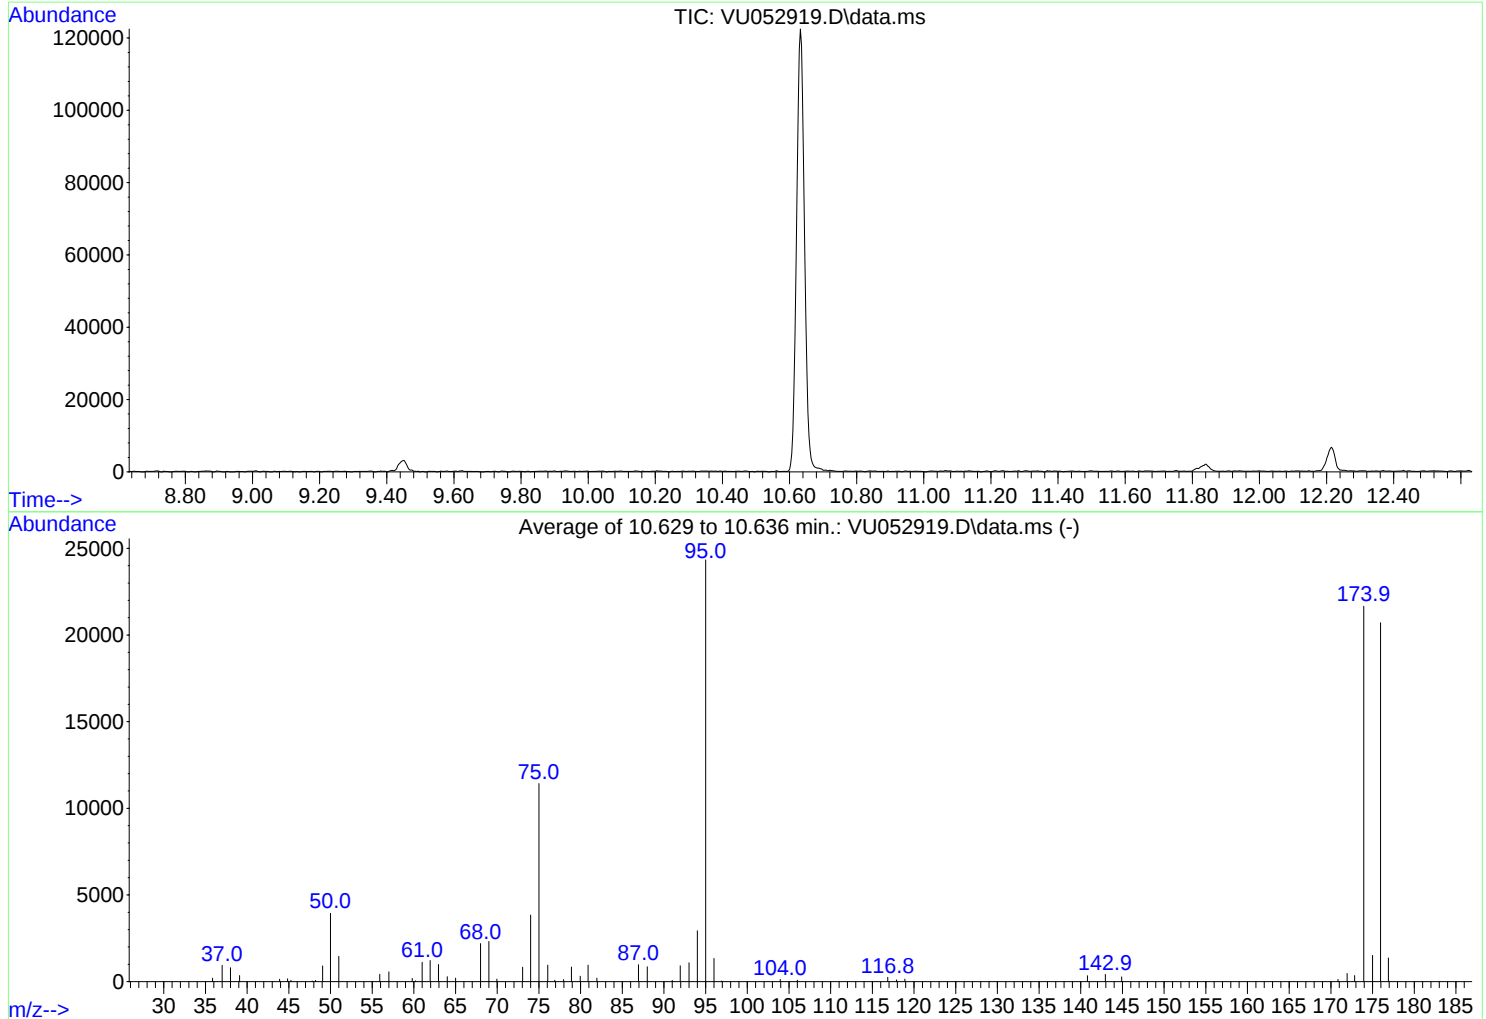

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	3944	PASS
75	95	30	80	46.9	11425	PASS
95	95	100	100	100.0	24336	PASS
96	95	5	9	5.5	1338	PASS
173	174	0.00	2	1.6	347	PASS
174	95	50	120	89.0	21653	PASS
175	174	5	9	7.0	1515	PASS
176	174	95	101	95.6	20707	PASS
177	176	5	9	6.6	1364	PASS

m/z	Abundance
43.90	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.90	182.0
37.00	990.0
38.00	747.0
39.10	379.0
44.00	241.0
44.90	188.0
47.80	106.0
48.20	116.0
49.10	841.0
50.00	3949.0
51.00	1278.0
55.90	459.0
57.00	556.0
59.90	216.0
61.00	1210.0
62.00	1252.0
62.90	998.0
64.00	347.0
65.00	207.0
68.00	2276.0
69.00	2373.0
70.00	162.0
73.00	818.0
74.00	3874.0
75.00	11496.0
76.10	1016.0
76.90	143.0
78.00	106.0
78.90	822.0
80.00	307.0
80.90	957.0
82.00	205.0
87.00	939.0
88.00	842.0
91.90	805.0
93.00	1025.0
94.00	2775.0
95.00	23808.0
96.00	1344.0
103.90	136.0
116.80	238.0
117.90	108.0
118.80	140.0
140.80	280.0
142.90	387.0
144.90	256.0
170.90	108.0
172.00	437.0
172.90	337.0
173.90	20888.0
175.00	1447.0
175.90	20224.0
176.90	1312.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.80	214.0
37.00	992.0
38.00	828.0
39.10	363.0
43.90	263.0
44.80	164.0
45.20	109.0
48.20	102.0
49.00	914.0
50.00	4071.0
51.00	1511.0
55.90	436.0
57.00	586.0
59.80	188.0
61.00	1132.0
62.00	1266.0
63.00	992.0
64.00	308.0
65.00	195.0
68.00	2249.0
69.00	2425.0
70.00	123.0
73.00	858.0
74.00	3928.0
75.00	11686.0
76.10	952.0
76.90	112.0
77.90	112.0
78.90	839.0
80.00	331.0
80.90	993.0
81.90	211.0
87.00	1035.0
88.00	930.0
91.00	107.0
92.00	947.0
93.00	1141.0
94.00	3066.0
95.00	25040.0
96.00	1317.0
96.90	115.0
104.00	125.0
106.00	114.0
116.80	246.0
117.90	107.0
118.90	150.0
140.80	375.0
142.90	429.0
144.90	301.0
170.80	130.0
171.90	518.0
172.80	354.0
173.90	22296.0
175.00	1613.0
175.90	21168.0
176.90	1388.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.90	208.0
37.00	840.0
38.00	831.0
39.10	311.0
43.90	270.0
44.80	158.0
45.30	108.0
49.00	971.0
50.00	3813.0
51.00	1583.0
55.90	393.0
57.00	563.0
59.70	157.0
60.20	144.0
61.00	1002.0
61.90	1151.0
63.00	976.0
64.00	207.0
65.00	205.0
68.00	2063.0
69.00	2163.0
69.90	151.0
73.10	818.0
74.00	3724.0
75.00	11093.0
76.00	873.0
77.90	142.0
78.90	869.0
79.90	311.0
80.90	915.0
81.90	197.0
86.90	964.0
88.00	803.0
91.00	103.0
91.90	991.0
93.00	1116.0
94.00	2979.0
95.00	24160.0
96.00	1353.0
104.00	114.0
106.00	123.0
116.90	256.0
117.90	101.0
119.00	161.0
140.80	367.0
143.00	421.0
144.90	281.0
170.80	137.0
171.90	467.0
172.90	349.0
174.00	21776.0
175.00	1486.0
176.00	20728.0
176.90	1392.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157