

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
 Data File : VU057785.D
 Acq On : 02 Feb 2024 10:16
 Operator : MD/SY
 Sample : VU0202WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0202WBL01

Quant Time: Feb 03 05:51:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Feb 02 00:27:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	41050	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	14627	0.941	ug/l	0.00
Spiked Amount 1.000			Recovery	=	94.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	11874	0.848	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057785.D
Acq On : 02 Feb 2024 10:16
Operator : MD/SY
Sample : VU0202WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0202WBL01

Quant Time: Feb 03 05:51:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Feb 02 00:27:55 2024
Response via : Initial Calibration




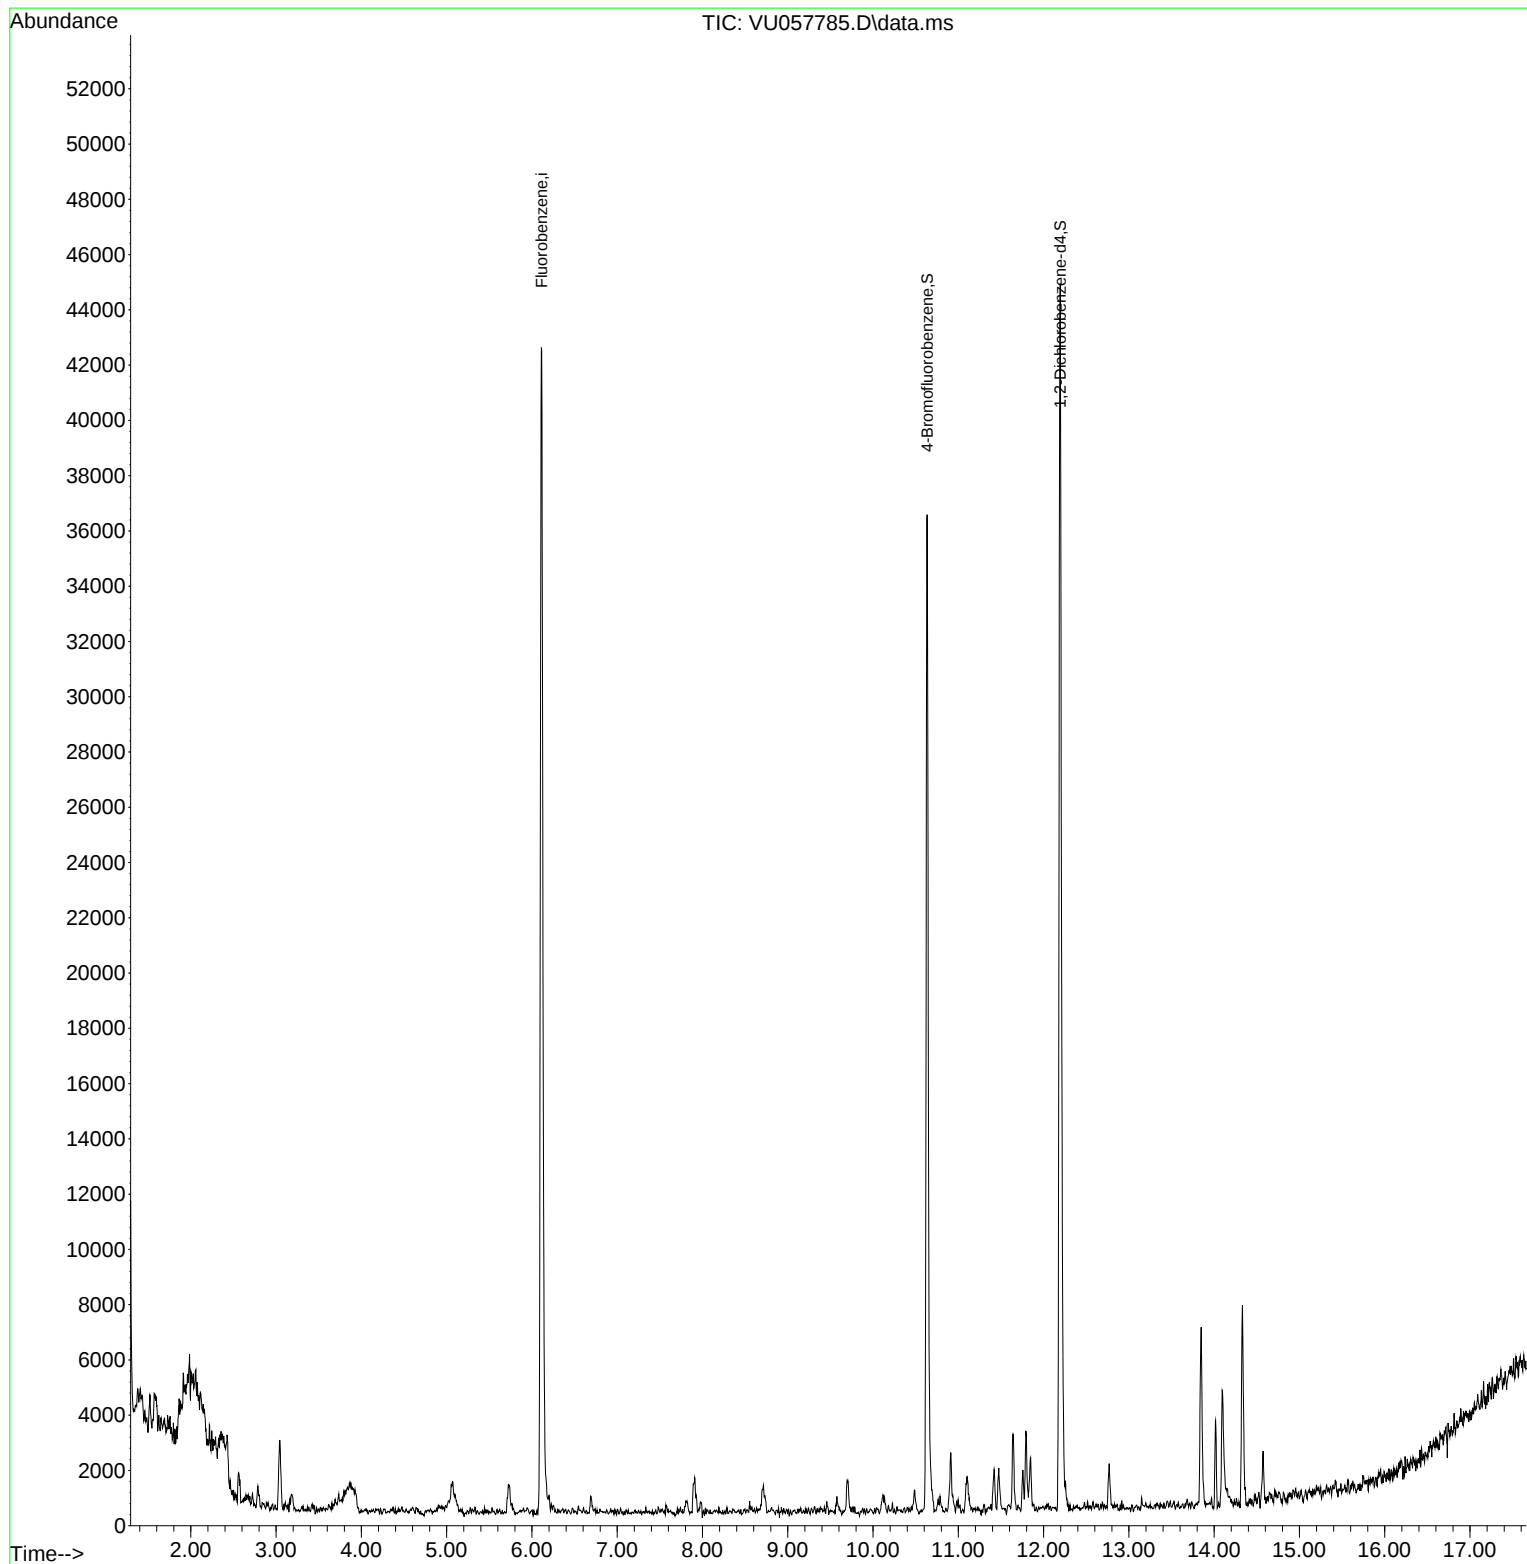


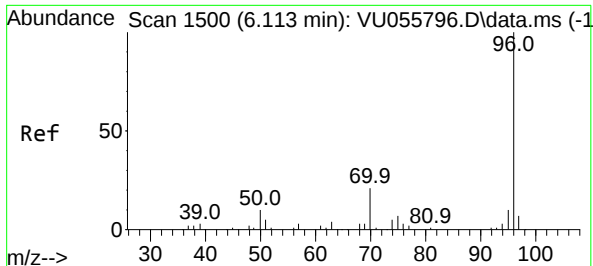

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU057785.D
Acq: 02 Feb 2024 10:16




Instrument :
MSVOA_U
ClientSampleId :
VU0202WBL01


Tgt Ion: 96	Resp: 41050
Ion Ratio	Lower Upper
96 100	
70 20.4	16.5 24.7
95 9.1	7.4 11.0
97 6.2	0.0 0.0#

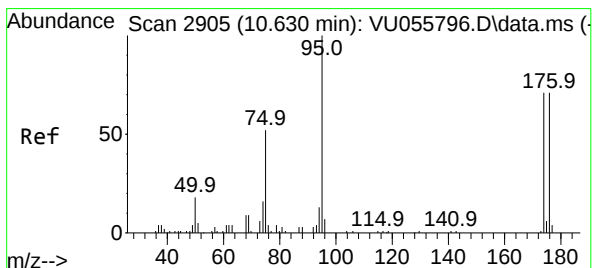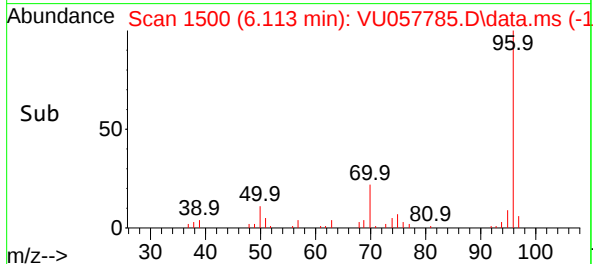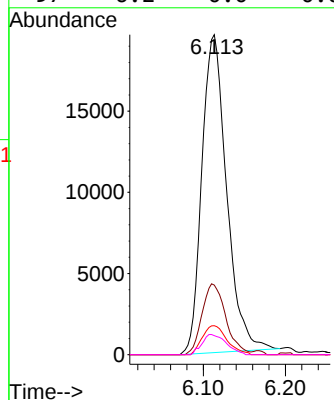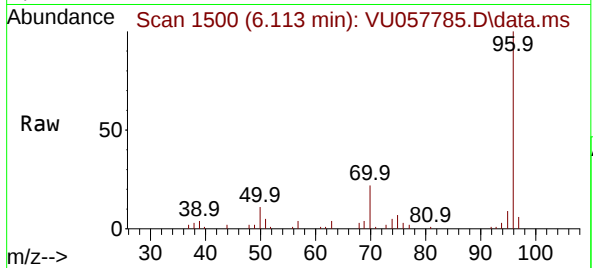

#57
4-Bromofluorobenzene
Concen: 0.941 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.004 min
Lab File: VU057785.D
Acq: 02 Feb 2024 10:16

Tgt Ion: 95	Resp: 14627
Ion Ratio	Lower Upper
95 100	
174 70.4	63.3 94.9
176 66.0	59.3 88.9

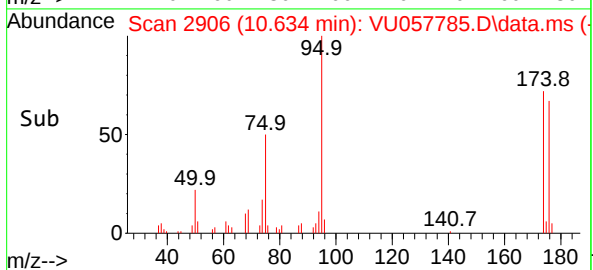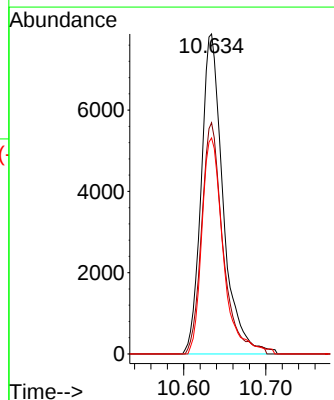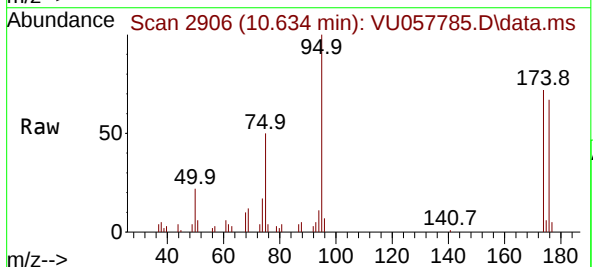

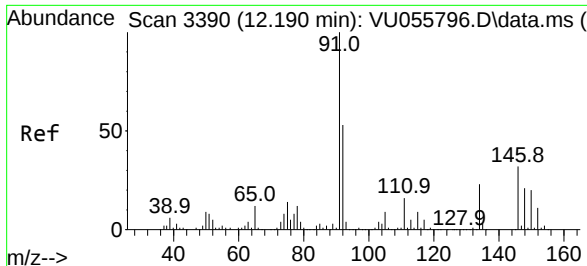

#68

1,2-Dichlorobenzene-d4

Concen: 0.848 ug/l

RT: 12.193 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU057785.D


Acq: 02 Feb 2024 10:16

Instrument :

MSVOA_U

ClientSampleId :

VU0202WBL01

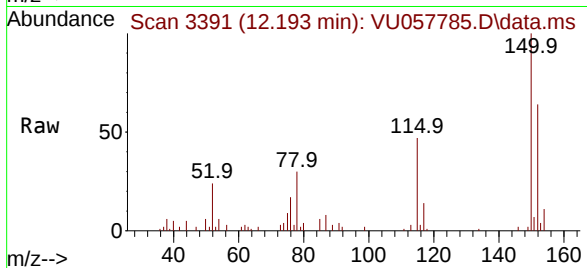

Tgt Ion:152 Resp: 11874

Ion Ratio Lower Upper

152 100

115 73.1 0.0 308.8

150 161.1 0.0 635.0

