

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
 Data File : VU057791.D
 Acq On : 02 Feb 2024 13:23
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Feb 03 05:55:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Feb 02 00:27:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	48377	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	16145	0.881	ug/l	0.00
Spiked Amount	1.000		Recovery	=	88.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	14395	0.873	ug/l	0.00
Spiked Amount	1.000		Recovery	=	87.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057791.D
Acq On : 02 Feb 2024 13:23
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Feb 03 05:55:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Feb 02 00:27:55 2024
Response via : Initial Calibration

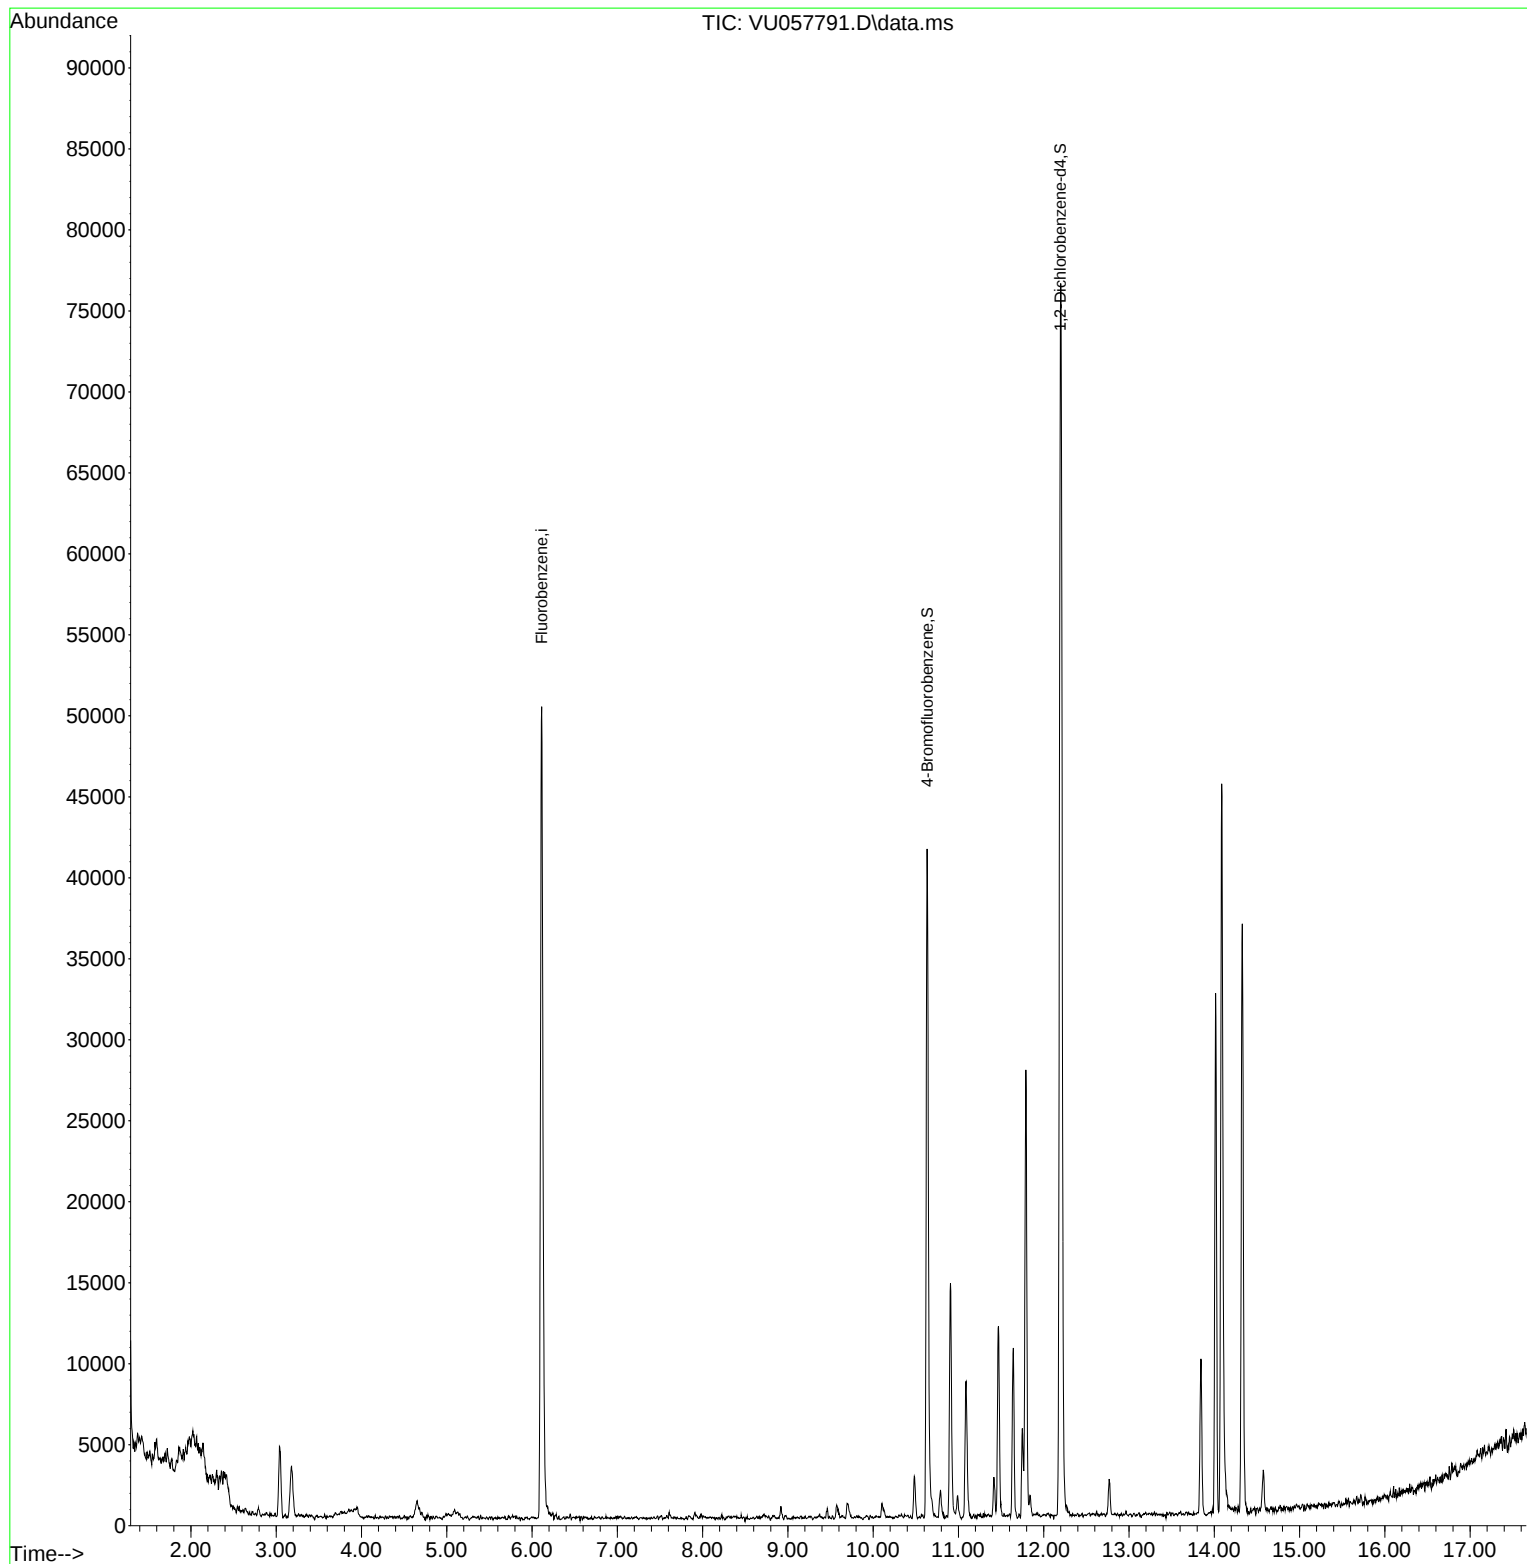




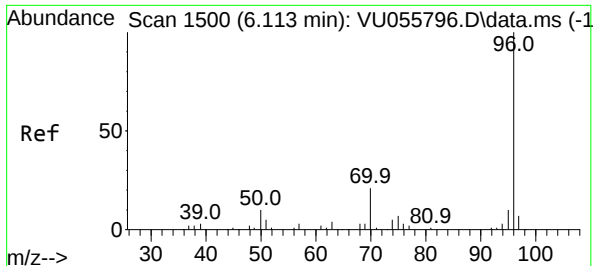


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU057791.D
Acq: 02 Feb 2024 13:23

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Tgt Ion: 96 Resp: 48377




Ion	Ratio	Lower	Upper
96	100		
70	19.3	16.5	24.7
95	9.1	7.4	11.0
97	6.3	0.0	0.0

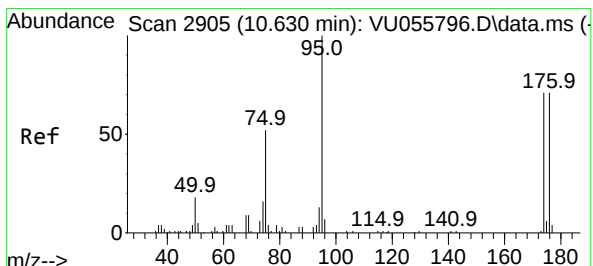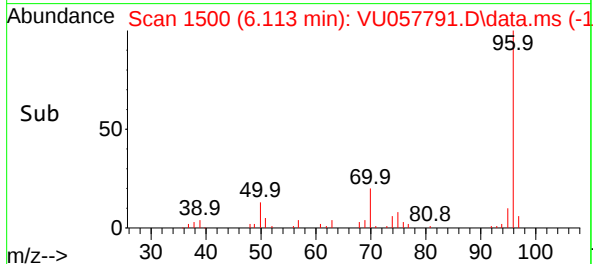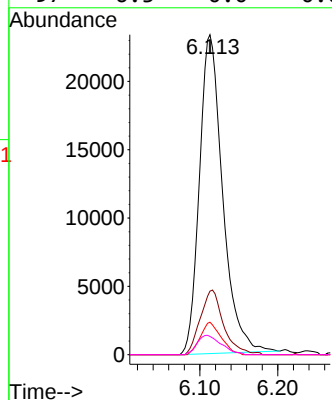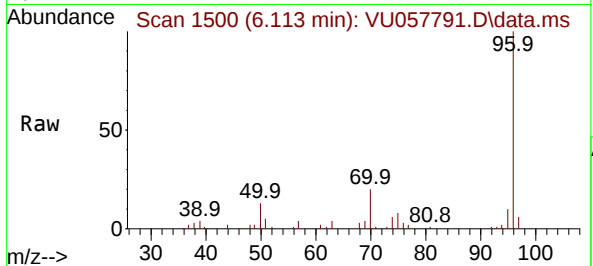


#57
4-Bromofluorobenzene
Concen: 0.881 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.004 min
Lab File: VU057791.D
Acq: 02 Feb 2024 13:23

Tgt Ion: 95 Resp: 16145

Ion	Ratio	Lower	Upper
95	100		
174	74.9	63.3	94.9
176	70.4	59.3	88.9

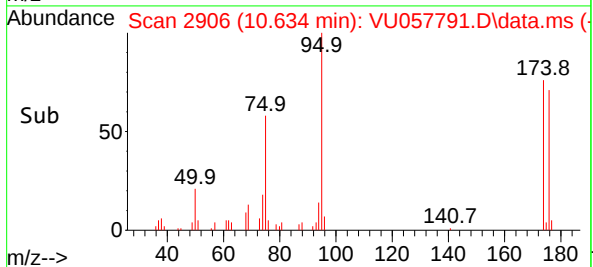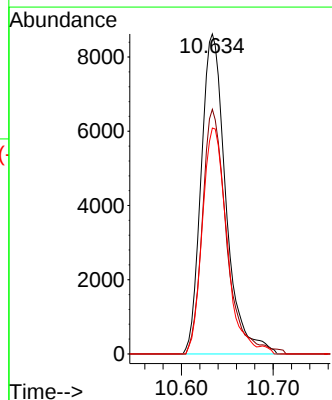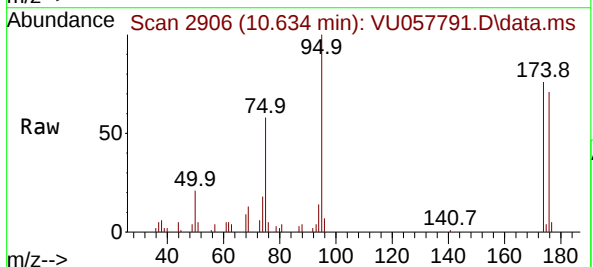

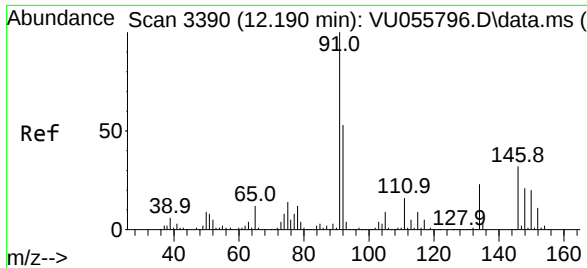

#68
1,2-Dichlorobenzene-d4
Concen: 0.873 ug/l
RT: 12.193 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU057791.D
Acq: 02 Feb 2024 13:23

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Tgt Ion:152 Resp: 14395
Ion Ratio Lower Upper
152 100
115 76.2 0.0 308.8
150 158.2 0.0 635.0

