

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
 Data File : VU057785.D
 Acq On : 02 Feb 2024 10:16
 Operator : MD/SY
 Sample : VU0202WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0202WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU057785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.001	219	221	225	rBV4	1043	951	1.07%	0.299%
2	2.560	390	395	398	rBV3	1095	1313	1.48%	0.413%
3	2.785	458	465	469	rBV2	785	985	1.11%	0.310%
4	3.043	535	545	557	rBV4	2538	4538	5.13%	1.426%
5	3.181	584	588	597	rVB4	545	905	1.02%	0.284%
6	3.924	817	819	830	rVB2	682	951	1.07%	0.299%
7	6.110	1486	1499	1521	rBV	42223	88484	100.00%	27.808%
8	7.907	2049	2058	2062	rBV3	1279	2266	2.56%	0.712%
9	9.695	2605	2614	2616	rBV3	1097	1133	1.28%	0.356%
10	10.116	2732	2745	2748	rBV4	689	1180	1.33%	0.371%
11	10.486	2851	2860	2870	rBV2	729	1137	1.28%	0.357%
12	10.634	2894	2906	2923	rBV2	35973	62291	70.40%	19.576%
13	10.910	2979	2992	2998	rBV4	2127	3433	3.88%	1.079%
14	11.100	3040	3051	3056	rBV5	1309	2427	2.74%	0.763%
15	11.418	3141	3150	3160	rBV3	1487	2349	2.65%	0.738%
16	11.473	3160	3167	3176	rBV3	1489	2275	2.57%	0.715%
17	11.640	3210	3219	3232	rVB3	2730	4327	4.89%	1.360%
18	11.756	3247	3255	3260	rBV3	1496	1987	2.25%	0.624%
19	11.791	3260	3266	3275	rVV2	2803	4163	4.70%	1.308%
20	11.846	3275	3283	3289	rVB4	1713	2580	2.92%	0.811%
21	12.193	3379	3391	3408	rBV2	44426	87727	99.14%	27.570%
22	12.769	3562	3570	3578	rBV2	1616	2402	2.71%	0.755%
23	13.846	3896	3905	3918	rVB5	6359	10047	11.35%	3.157%
24	14.016	3951	3958	3964	rBV6	3193	3802	4.30%	1.195%
25	14.094	3973	3982	3996	rBV3	4236	8300	9.38%	2.608%
26	14.332	4047	4056	4065	rBV4	7337	11872	13.42%	3.731%
27	14.573	4120	4131	4138	rBV2	2068	3215	3.63%	1.010%
28	16.743	4803	4806	4809	rBV4	1258	1157	1.31%	0.364%




Sum of corrected areas: 318197

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057785.D
Acq On : 02 Feb 2024 10:16
Operator : MD/SY
Sample : VU0202WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0202WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

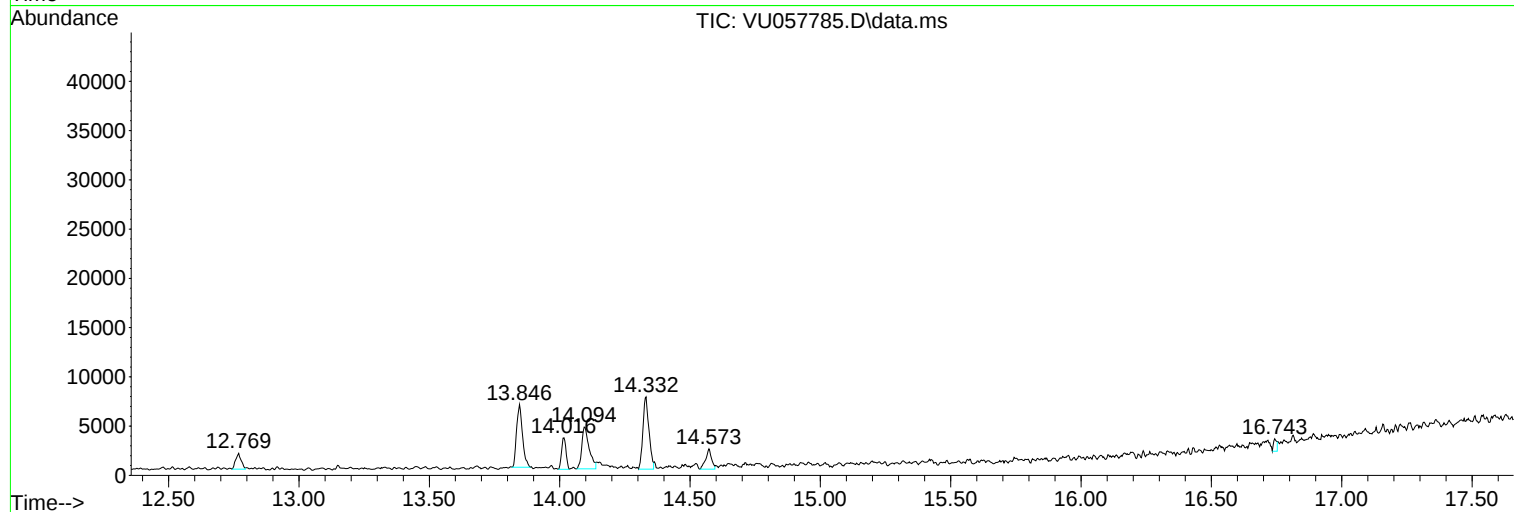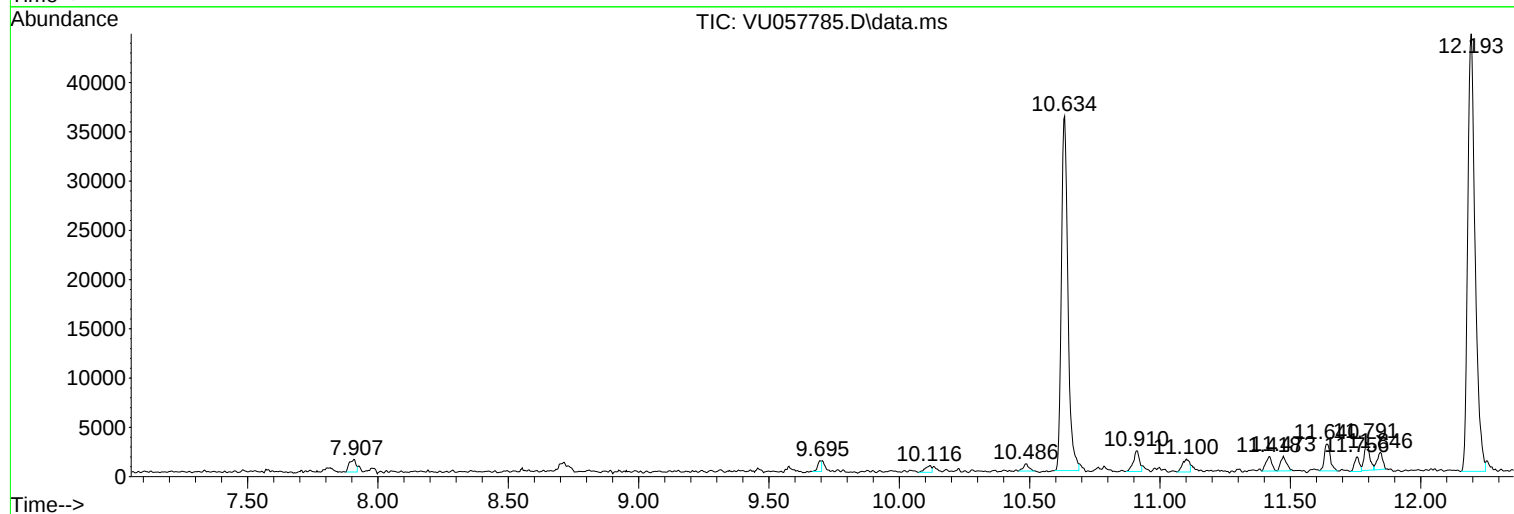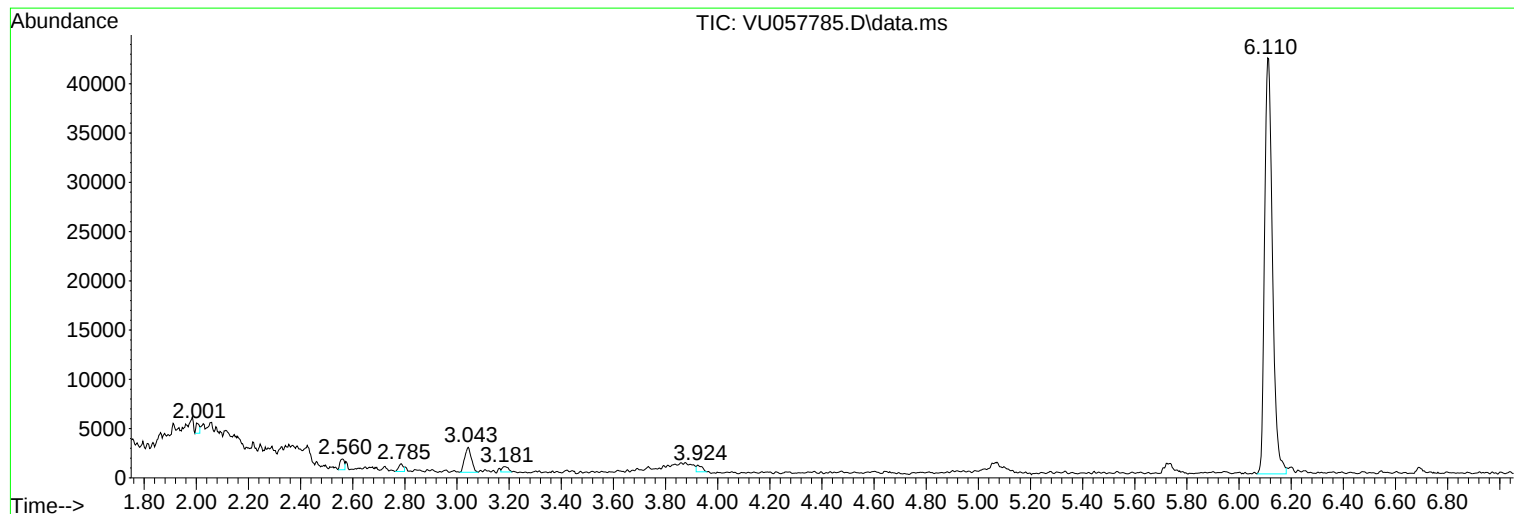

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057785.D
Acq On : 02 Feb 2024 10:16
Operator : MD/SY
Sample : VU0202WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0202WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057785.D
Acq On : 02 Feb 2024 10:16
Operator : MD/SY
Sample : VU0202WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0202WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------