

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
 Data File : VU057788.D
 Acq On : 02 Feb 2024 11:43
 Operator : MD/SY
 Sample : P1174-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU057788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.576	387	400	416	rBV	563578	917394	25.72%	4.133%
2	3.039	530	544	574	rBV	288374	563458	15.80%	2.538%
3	3.348	625	640	671	rBV	434366	873030	24.48%	3.933%
4	4.660	1029	1048	1077	rBV	293810	675857	18.95%	3.045%
5	5.309	1232	1250	1270	rBV	452651	1011886	28.37%	4.558%
6	5.518	1298	1315	1336	rBV	333217	728093	20.41%	3.280%
7	5.769	1377	1393	1421	rBV	537300	1176205	32.98%	5.298%
8	6.110	1488	1499	1517	rBV	45226	91027	2.55%	0.410%
9	6.537	1618	1632	1662	rBV	357638	677940	19.01%	3.054%
10	6.785	1695	1709	1738	rBV	588170	1109853	31.12%	5.000%
11	7.965	2060	2076	2103	rBV	239796	420868	11.80%	1.896%
12	8.396	2198	2210	2229	rBV	283288	489273	13.72%	2.204%
13	8.550	2246	2258	2280	rVB	126194	214330	6.01%	0.965%
14	9.441	2522	2535	2561	rBV	796784	1323787	37.12%	5.963%
15	9.566	2561	2574	2599	rVV	1712843	2741032	76.86%	12.347%
16	9.688	2599	2612	2646	rVB	1405489	2371296	66.49%	10.682%
17	10.097	2724	2739	2773	rBV4	1796940	3566488	100.00%	16.066%
18	10.631	2895	2905	2923	rBV2	41589	70420	1.97%	0.317%
19	11.833	3269	3279	3301	rVB	205411	333166	9.34%	1.501%
20	12.206	3379	3395	3427	rBV	1023443	1714978	48.09%	7.725%
21	13.836	3888	3902	3935	rBV	694258	1128879	31.65%	5.085%




Sum of corrected areas: 22199260

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057788.D
Acq On : 02 Feb 2024 11:43
Operator : MD/SY
Sample : P1174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

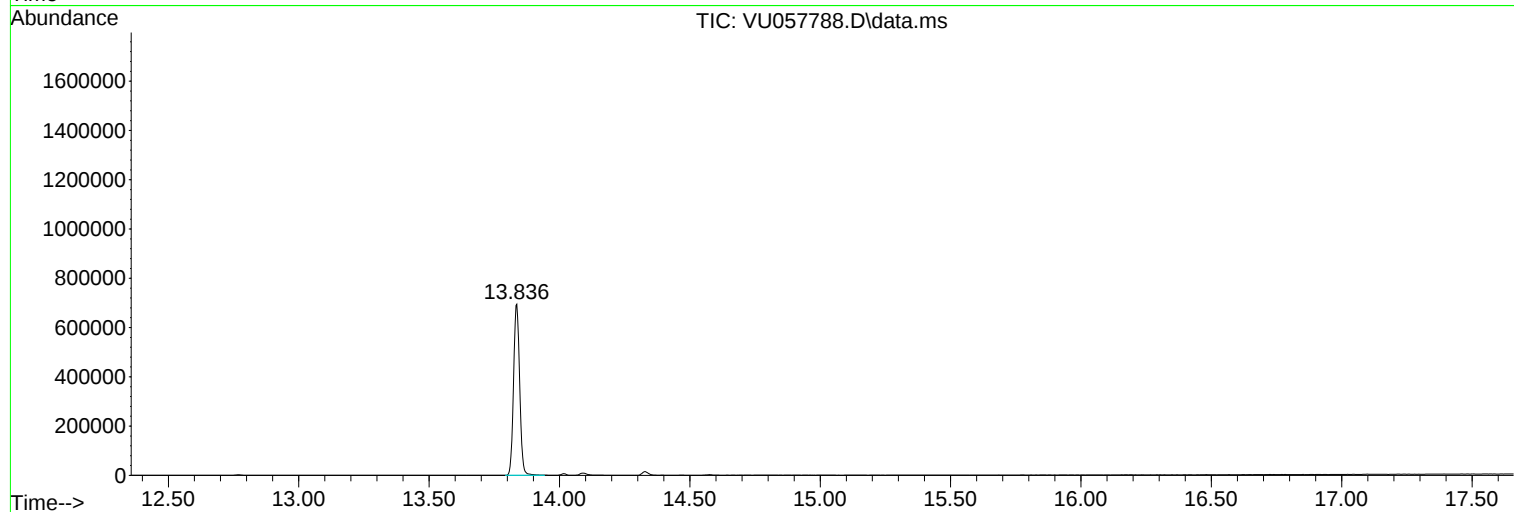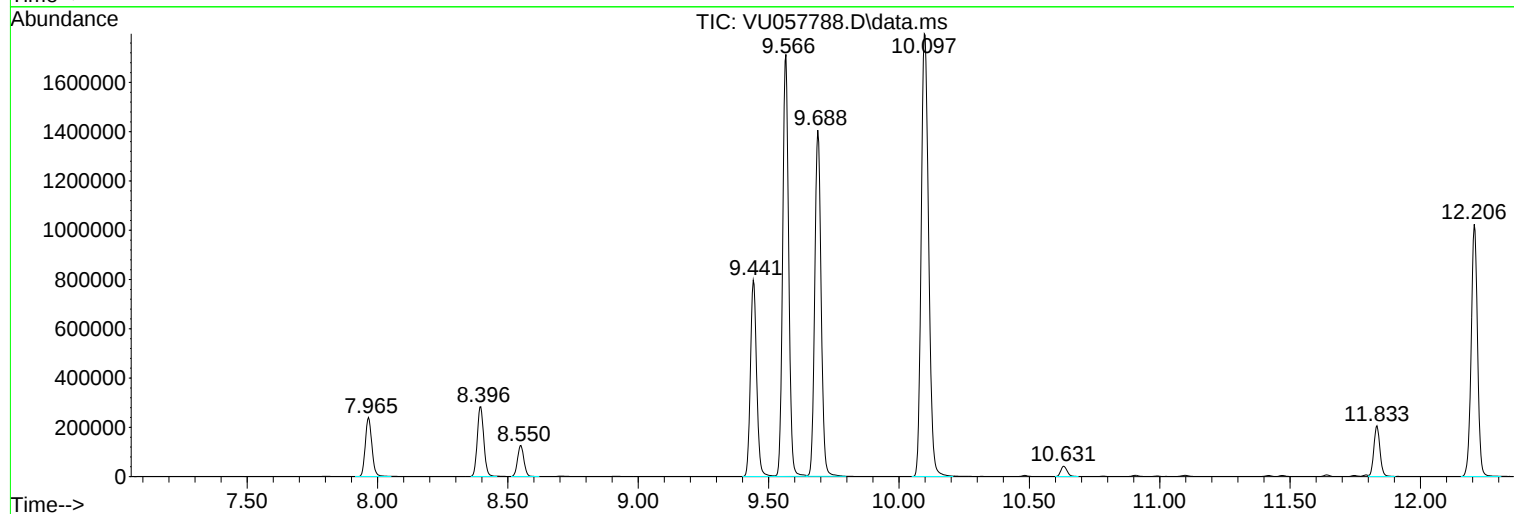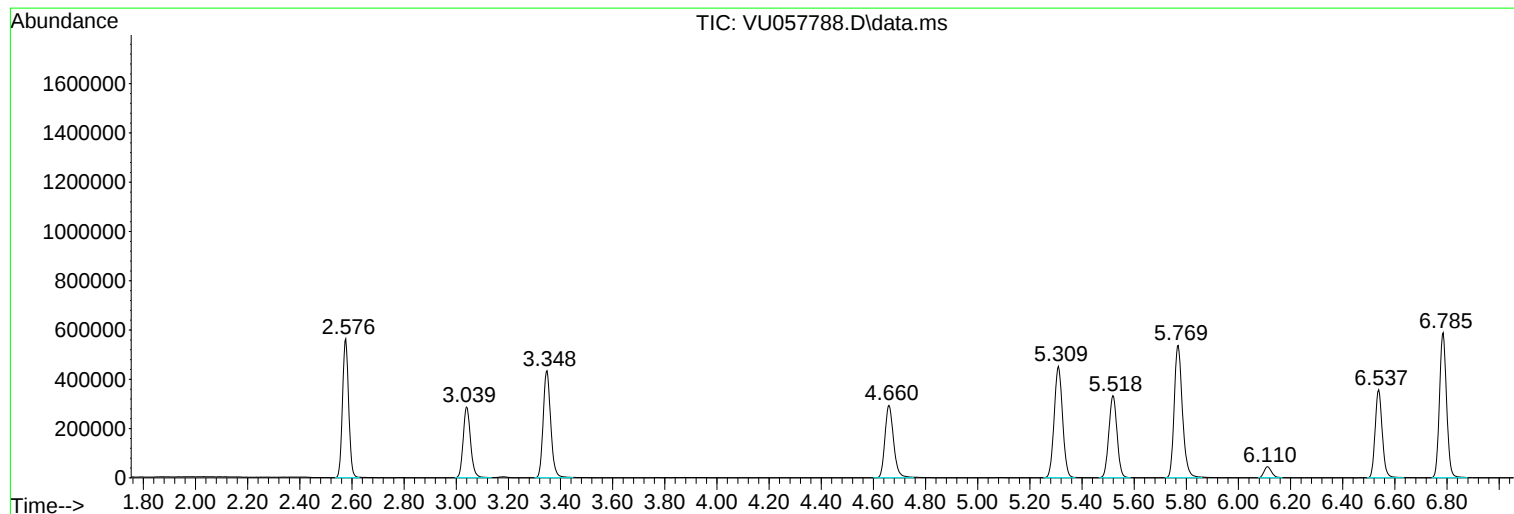

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057788.D
Acq On : 02 Feb 2024 11:43
Operator : MD/SY
Sample : P1174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057788.D
Acq On : 02 Feb 2024 11:43
Operator : MD/SY
Sample : P1174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------