

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
 Data File : VU057790.D
 Acq On : 02 Feb 2024 12:35
 Operator : MD/SY
 Sample : P1174-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU057790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.856	166	176	192	rBV	240123	309412	11.71%	1.049%
2	2.136	251	263	281	rVB	1360453	1995710	75.52%	6.765%
3	3.354	623	642	677	rBV	1124455	2601695	98.46%	8.819%
4	3.862	780	800	827	rBV	310287	747221	28.28%	2.533%
5	4.657	1028	1047	1074	rBV2	180081	452599	17.13%	1.534%
6	4.965	1126	1143	1166	rBV	223463	500881	18.95%	1.698%
7	5.521	1303	1316	1338	rBV	146908	305568	11.56%	1.036%
8	6.110	1485	1499	1520	rBV2	42328	88456	3.35%	0.300%
9	6.914	1737	1749	1780	rBV	170488	333727	12.63%	1.131%
10	7.602	1948	1963	1992	rBV	463692	830523	31.43%	2.815%
11	8.206	2139	2151	2177	rBV	220299	383070	14.50%	1.298%
12	8.570	2249	2264	2294	rBV	194552	345271	13.07%	1.170%
13	9.528	2549	2562	2584	rBV	304669	508326	19.24%	1.723%
14	10.479	2845	2858	2881	rBV	560377	872366	33.01%	2.957%
15	10.631	2895	2905	2923	rVB	44967	72224	2.73%	0.245%
16	10.778	2938	2951	2960	rBV	362907	613206	23.21%	2.079%
17	10.901	2976	2989	3003	rBV	1439772	2215765	83.85%	7.511%
18	10.981	3003	3014	3032	rVV	333128	534929	20.24%	1.813%
19	11.084	3032	3046	3068	rVV2	1657944	2642509	100.00%	8.957%
20	11.412	3136	3148	3155	rBV	244347	391082	14.80%	1.326%
21	11.460	3155	3163	3187	rVB	1460066	2241731	84.83%	7.599%
22	11.637	3198	3218	3235	rBV	585743	897824	33.98%	3.043%
23	11.740	3238	3250	3257	rBV	508753	817163	30.92%	2.770%
24	11.788	3257	3265	3289	rVB	1679670	2547970	96.42%	8.637%
25	12.203	3376	3394	3429	rBV	1598884	2445582	92.55%	8.290%
26	13.836	3885	3902	3918	rBV4	36614	65558	2.48%	0.222%
27	14.016	3945	3958	3968	rBV	1126679	1731920	65.54%	5.871%
28	14.081	3968	3978	4000	rVB	665663	1063481	40.25%	3.605%
29	14.325	4041	4054	4075	rBV	580425	945449	35.78%	3.205%




Sum of corrected areas: 29501218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057790.D
Acq On : 02 Feb 2024 12:35
Operator : MD/SY
Sample : P1174-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

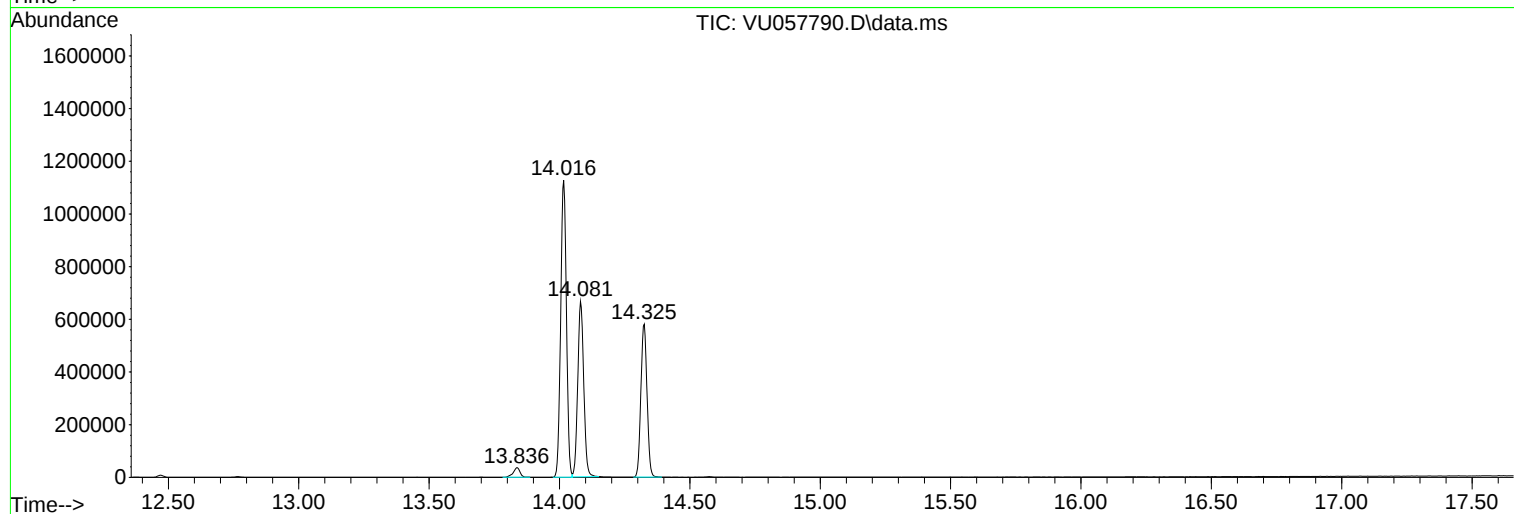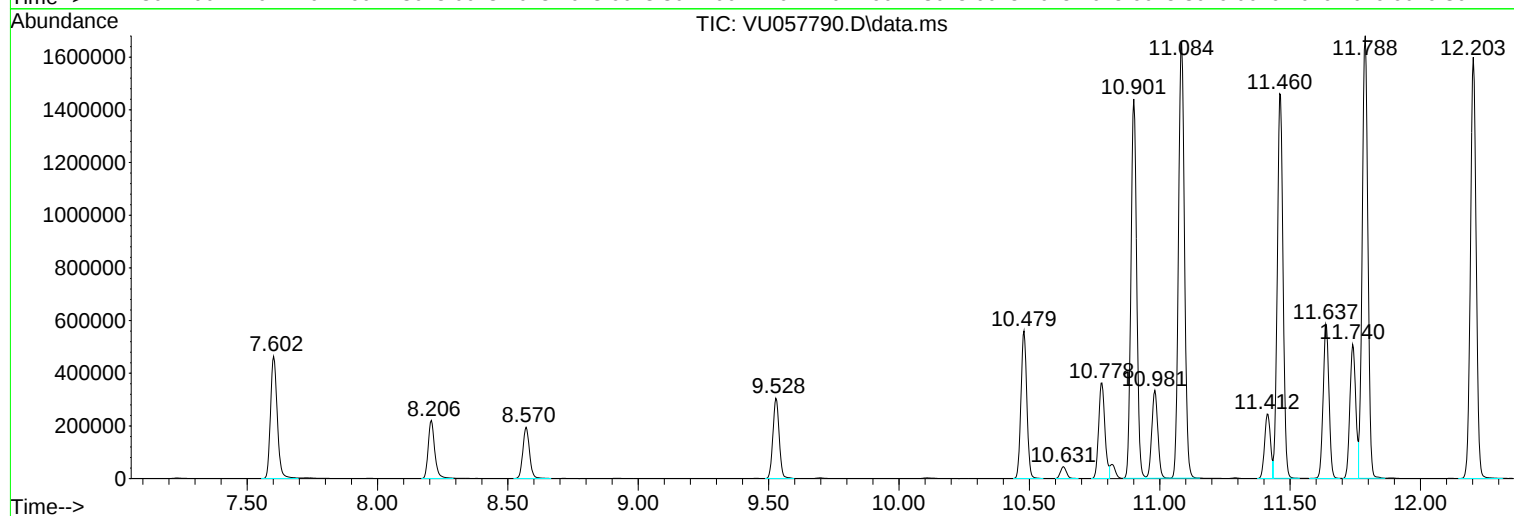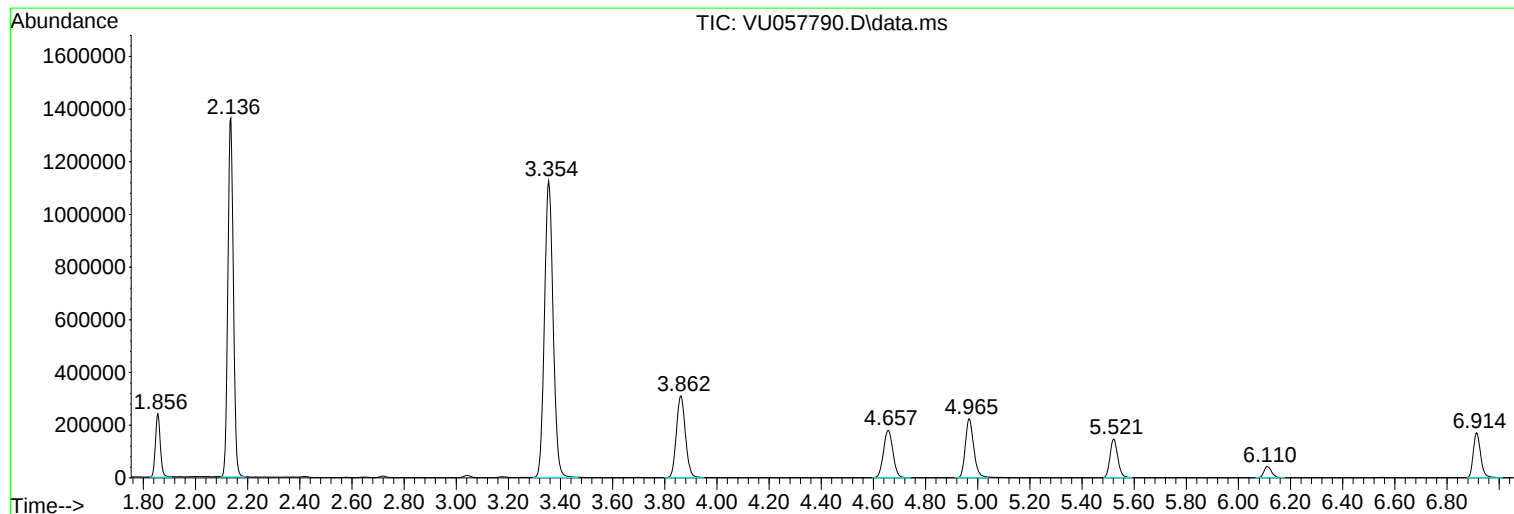

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057790.D
Acq On : 02 Feb 2024 12:35
Operator : MD/SY
Sample : P1174-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057790.D
Acq On : 02 Feb 2024 12:35
Operator : MD/SY
Sample : P1174-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------