


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020224\
Data File : VU057783.D
Acq On : 02 Feb 2024 08:47
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U013124DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Feb 02 00:27:55 2024

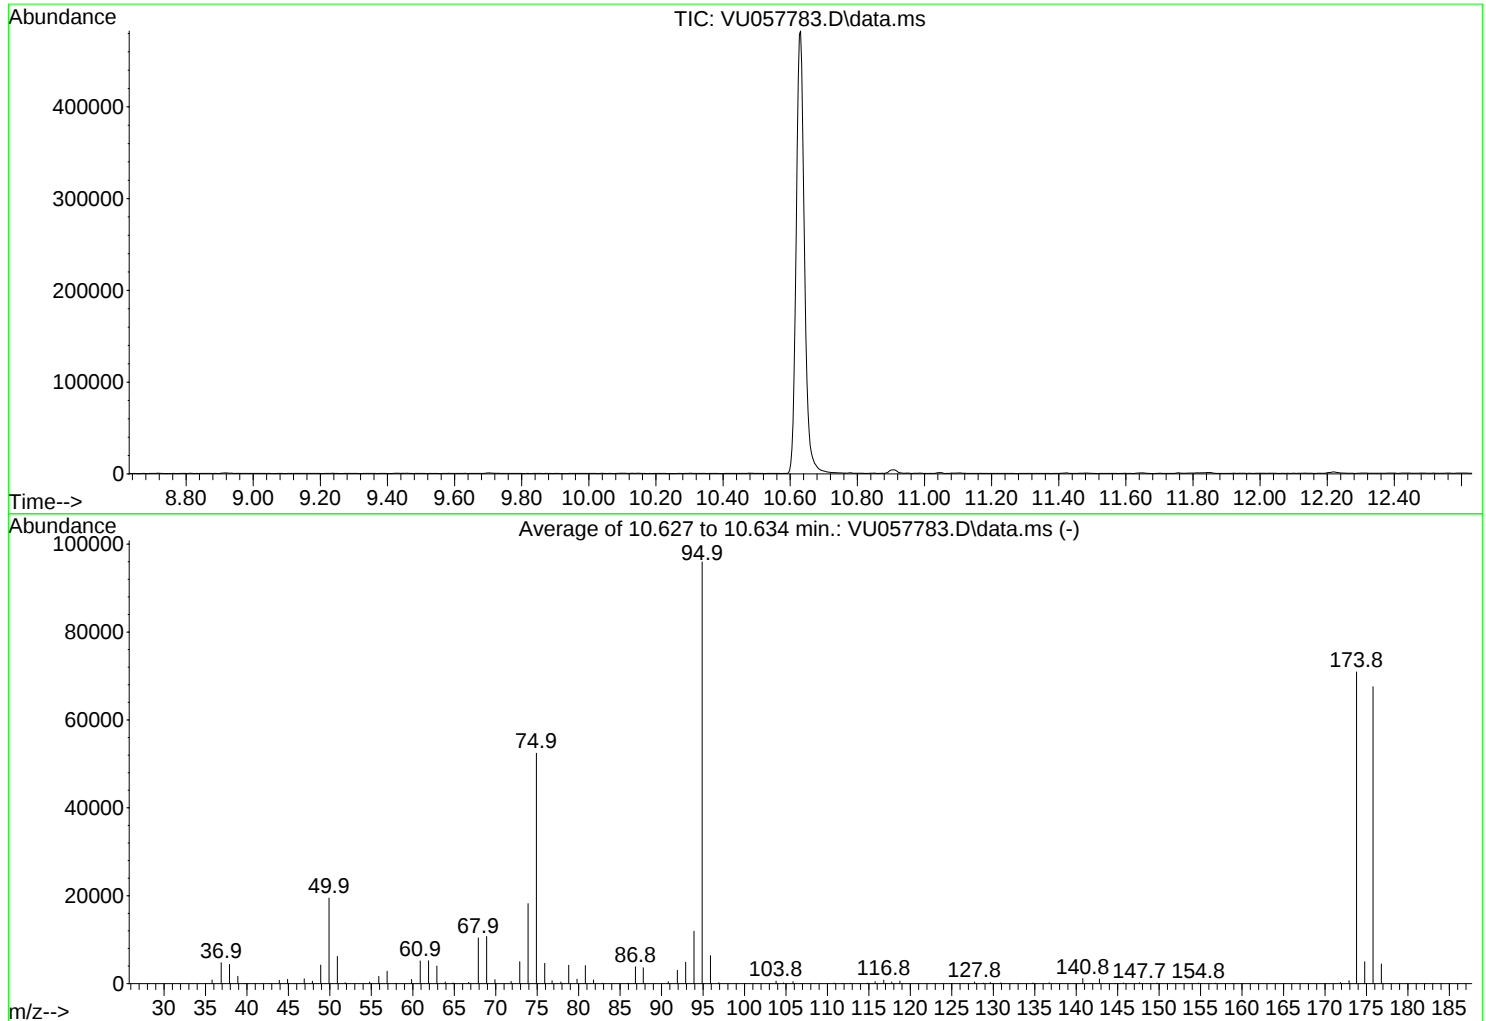

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	19469	PASS
75	95	30	60	54.6	52424	PASS
95	95	100	100	100.0	95973	PASS
96	95	5	9	6.6	6372	PASS
173	174	0.00	2	1.0	690	PASS
174	95	50	100	73.9	70907	PASS
175	174	5	9	7.0	4991	PASS
176	174	95	101	95.3	67584	PASS
177	176	5	9	6.6	4485	PASS