


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU020320\
 Data File : VU036668.D
 Acq On : 03 Feb 2020 10:13
 Operator : JC/MD
 Sample : BFB47
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Title : VOC Analysis
 Last Update : Mon Jan 27 00:51:24 2020

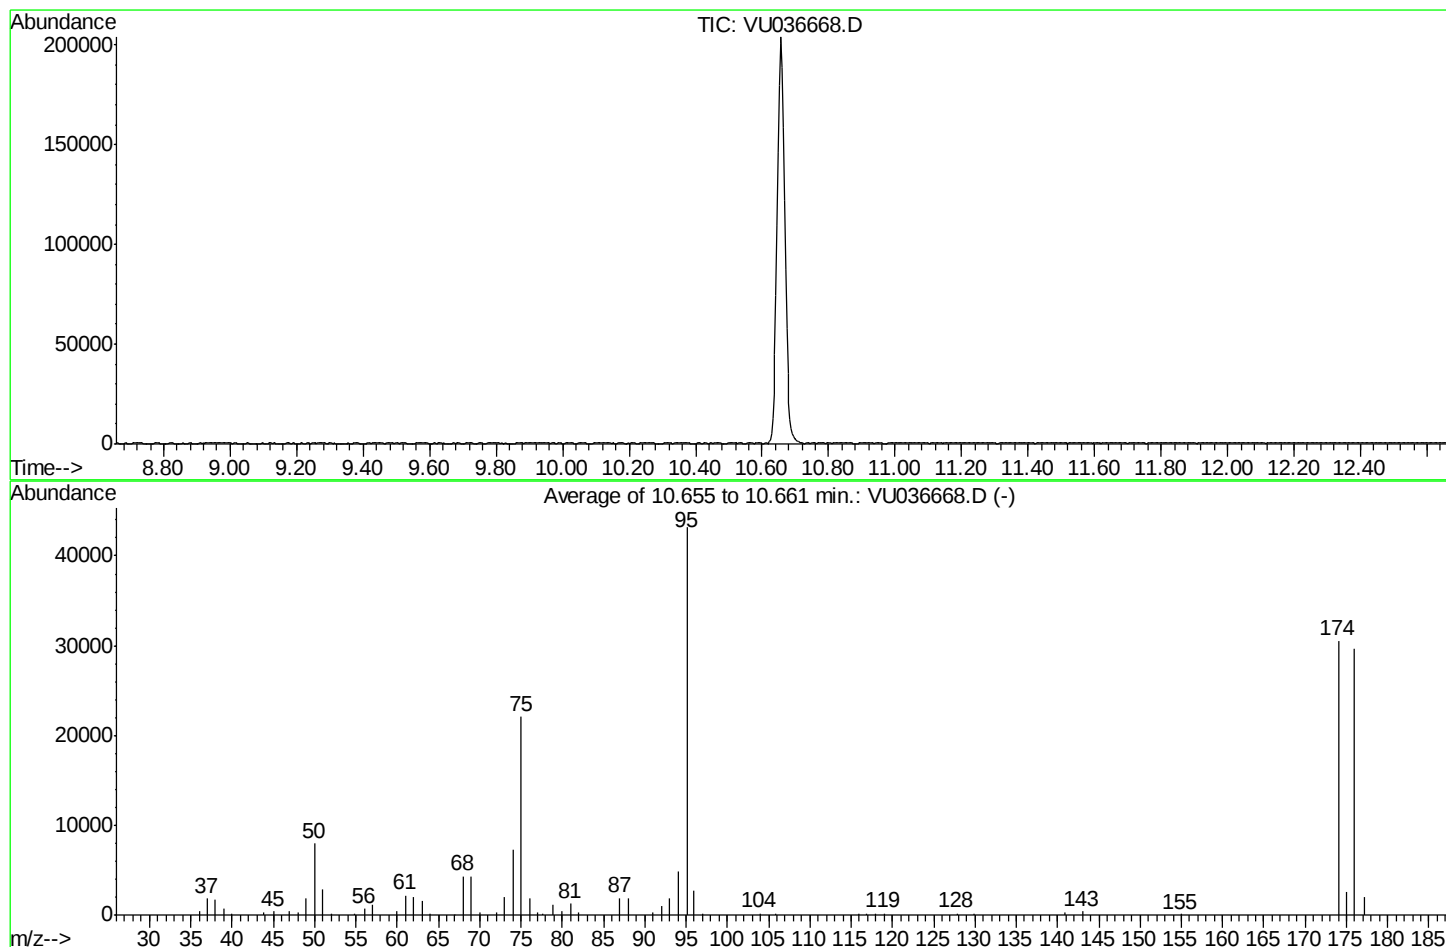

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	7943	PASS
75	95	30	80	51.1	22053	PASS
95	95	100	100	100.0	43184	PASS
96	95	5	9	6.1	2647	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.7	30522	PASS
175	174	5	9	8.2	2516	PASS
176	174	95	101	97.0	29594	PASS
177	176	5	9	6.6	1953	PASS

m/z	Abundance
36.00	389.0
37.00	1874.0
38.00	1788.0
39.00	717.0
40.10	108.0
44.00	522.0
45.00	441.0
46.90	531.0
48.00	317.0
49.00	1905.0
50.00	8185.0
51.00	2751.0
52.00	130.0
54.90	121.0
56.00	695.0
57.00	1063.0
60.00	454.0
61.00	2294.0
62.00	2135.0
63.00	1643.0
64.00	152.0
66.90	110.0
68.00	4387.0
69.00	4340.0
70.00	360.0
72.00	288.0
73.00	2070.0
74.10	7374.0
75.00	22808.0
76.00	1941.0
77.00	358.0
77.70	125.0
78.90	1216.0
79.90	485.0
81.00	1207.0
81.90	273.0
87.00	1997.0
88.00	1777.0
90.90	226.0
92.00	1030.0
93.00	1764.0
94.10	4786.0
95.10	43592.0
96.00	2803.0
97.00	166.0
103.90	127.0
106.00	145.0
116.90	196.0
118.00	108.0
119.00	217.0
127.90	166.0
129.90	117.0
140.90	382.0
143.00	398.0
155.00	134.0
174.00	30240.0
175.00	2537.0
176.00	30024.0
177.10	1993.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	412.0
37.00	1835.0
38.00	1738.0
39.00	676.0
40.00	109.0
43.90	569.0
45.00	396.0
46.90	499.0
48.00	291.0
49.00	1886.0
50.00	8188.0
51.00	2938.0
52.00	126.0
54.90	135.0
56.00	679.0
57.00	1134.0
60.00	500.0
61.00	2305.0
62.00	2146.0
63.00	1569.0
64.00	129.0
68.00	4412.0
69.00	4366.0
70.00	361.0
72.00	317.0
73.00	2071.0
74.10	7511.0
75.10	22680.0
76.00	1913.0
76.90	347.0
77.70	116.0
78.90	1255.0
79.90	436.0
81.00	1262.0
82.00	284.0
87.00	1989.0
88.00	1865.0
91.00	243.0
92.10	1061.0
93.00	1873.0
94.10	4967.0
95.10	44488.0
96.00	2682.0
97.00	142.0
103.90	159.0
105.90	150.0
115.90	120.0
116.90	196.0
118.00	126.0
119.00	220.0
127.80	175.0
129.90	130.0
141.00	363.0
143.00	396.0
154.90	139.0
174.00	31616.0
175.00	2630.0
176.00	30560.0
177.10	2032.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	393.0
37.00	1688.0
38.00	1501.0
39.00	595.0
39.90	101.0
43.90	643.0
45.00	311.0
46.90	413.0
48.00	246.0
49.00	1692.0
50.00	7457.0
51.00	2705.0
56.00	614.0
57.00	1084.0
59.90	475.0
61.00	2024.0
62.00	1898.0
63.00	1444.0
64.00	135.0
68.00	4042.0
69.00	4113.0
70.00	335.0
72.00	292.0
73.00	1927.0
74.10	7092.0
75.10	20672.0
76.00	1716.0
76.90	260.0
77.70	100.0
78.90	1163.0
80.00	390.0
81.00	1191.0
81.90	251.0
87.00	1741.0
88.00	1731.0
91.00	214.0
92.00	1048.0
93.00	1767.0
94.10	4698.0
95.10	41472.0
96.00	2458.0
97.00	113.0
104.00	176.0
105.80	147.0
115.90	126.0
116.90	174.0
118.00	133.0
119.00	191.0
127.80	148.0
129.90	130.0
141.00	299.0
143.00	345.0
154.90	120.0
174.00	29712.0
175.00	2381.0
176.00	28200.0
177.10	1836.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
43.90	329.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47