
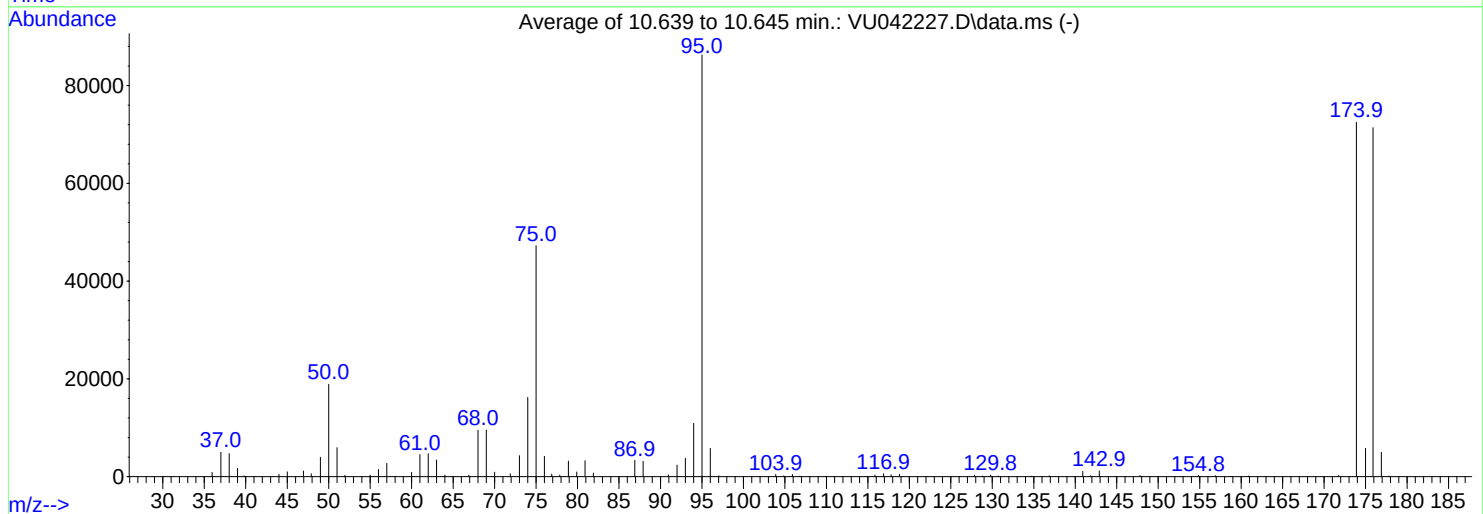


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020321\
Data File : VU042227.D
Acq On : 03 Feb 2021 11:09
Operator : SY/MD
Sample : BFB42
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR012021WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Feb 05 02:23:43 2021

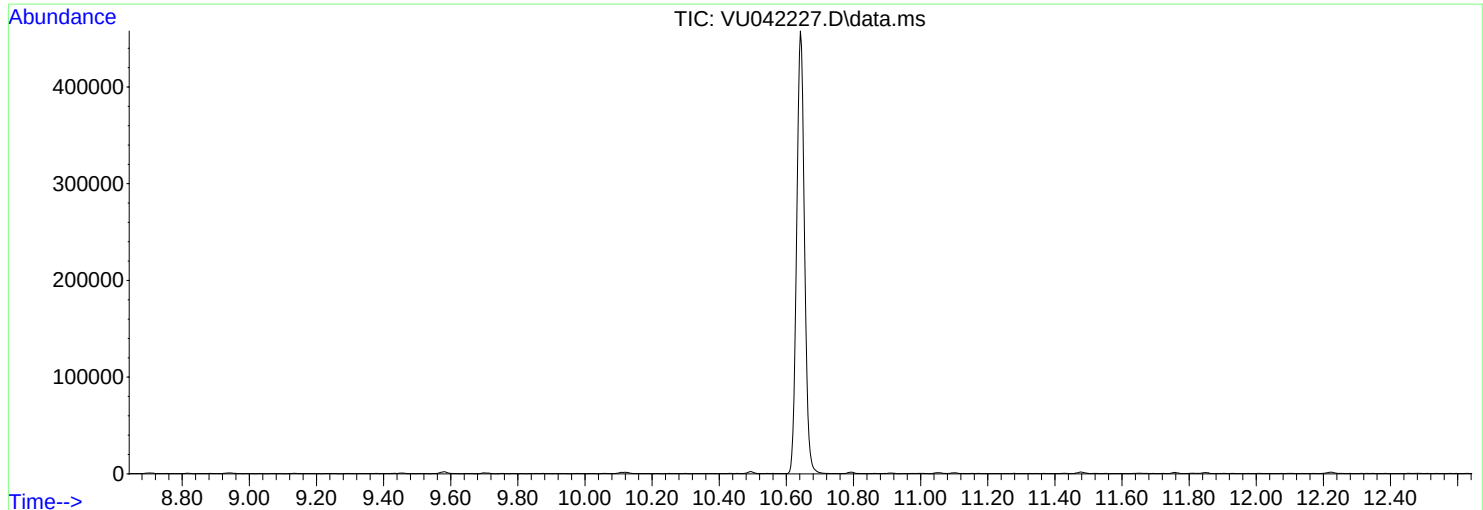

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	18888	PASS
75	95	30	80	54.7	47235	PASS
95	95	100	100	100.0	86288	PASS
96	95	5	9	6.7	5796	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	72509	PASS
175	174	5	9	7.9	5760	PASS
176	174	95	101	98.5	71395	PASS
177	176	5	9	7.0	4995	PASS

m/z	Abundance
35.90	853.0
37.00	5154.0
38.00	4662.0
39.00	1712.0
39.80	156.0
44.00	847.0
45.00	971.0
47.00	1220.0
47.90	583.0
49.00	3983.0
50.00	18672.0
51.00	5777.0
51.90	218.0
55.00	323.0
56.00	1438.0
57.00	2731.0
58.00	155.0
60.00	903.0
61.00	4497.0
62.00	4782.0
63.00	3367.0
64.00	368.0
66.90	321.0
68.00	9301.0
69.00	9274.0
70.00	876.0
71.90	492.0
73.00	4241.0
74.00	16091.0
75.00	46648.0
76.00	4189.0
76.90	537.0
77.80	335.0
78.90	3060.0
79.90	957.0
80.90	3182.0
81.90	736.0
86.90	3205.0
87.90	3017.0
90.90	338.0
92.00	2270.0
93.00	3618.0
94.00	10950.0
95.00	84720.0
96.00	5724.0
97.10	167.0
103.90	441.0
104.80	147.0
105.90	436.0
106.80	101.0
111.80	105.0
115.80	302.0
116.90	569.0
117.80	343.0
118.80	510.0
127.90	261.0
128.80	193.0
129.80	305.0
130.70	110.0
136.90	168.0
140.90	984.0
141.80	187.0
142.90	1034.0
144.80	108.0
147.80	255.0
152.80	102.0
154.80	238.0
156.90	167.0
160.90	135.0
171.70	243.0
173.90	69160.0
175.00	5513.0
175.90	68384.0
176.90	4671.0
177.80	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	930.0
37.00	5121.0
38.00	4882.0
39.00	1735.0
39.80	185.0
43.00	103.0
44.00	845.0
45.00	1012.0
46.90	1214.0
47.90	596.0
49.00	4047.0
50.00	19488.0
51.00	6083.0
51.90	266.0
55.00	359.0
56.00	1533.0
57.00	2833.0
58.00	136.0
60.00	920.0
61.00	4641.0
62.00	4827.0
63.00	3473.0
64.00	364.0
66.90	325.0
68.00	9780.0
69.00	9728.0
70.00	975.0
71.90	613.0
73.00	4444.0
74.00	16688.0
75.00	48560.0
76.00	4288.0
76.90	545.0
77.90	328.0
78.90	3305.0
79.90	1011.0
80.90	3379.0
81.90	752.0
86.90	3400.0
87.90	3220.0
91.00	394.0
92.00	2402.0
93.00	3854.0
94.00	11191.0
95.00	88856.0
96.00	5978.0
97.10	185.0
103.90	462.0
104.90	172.0
105.90	466.0
106.80	105.0
112.90	105.0
114.70	107.0
115.90	327.0
116.90	593.0
117.80	398.0
118.80	522.0
127.90	328.0
128.80	145.0
129.80	340.0
130.70	133.0
134.70	134.0
136.90	184.0
139.90	100.0
140.90	1127.0
141.80	200.0
142.90	1221.0
144.80	101.0
147.80	272.0
154.90	261.0
156.90	221.0
160.90	122.0
171.70	250.0
173.90	74640.0
175.00	5936.0
175.90	73720.0
176.90	5167.0
177.80	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	863.0
37.00	4655.0
38.00	4572.0
39.00	1538.0
39.80	179.0
43.00	115.0
44.00	779.0
45.00	931.0
46.90	1038.0
47.90	557.0
49.00	3887.0
50.00	18504.0
51.00	5887.0
52.00	304.0
55.00	314.0
56.00	1458.0
57.00	2623.0
60.00	844.0
61.00	4401.0
62.00	4511.0
63.00	3366.0
64.00	310.0
66.90	263.0
68.00	9410.0
69.00	9550.0
70.00	947.0
71.90	636.0
73.00	4223.0
74.00	15809.0
75.00	46496.0
76.00	4002.0
76.90	538.0
77.90	275.0
78.90	3144.0
79.90	902.0
80.90	3229.0
81.90	687.0
86.90	3375.0
87.90	3157.0
91.00	387.0
92.00	2400.0
93.00	3829.0
94.00	10569.0
95.00	85288.0
96.00	5686.0
97.00	196.0
103.90	447.0
104.90	176.0
105.90	433.0
106.80	101.0
109.90	101.0
110.90	121.0
115.80	325.0
116.90	567.0
117.80	404.0
118.80	475.0
127.80	332.0
128.90	114.0
129.80	335.0
130.70	133.0
134.80	167.0
136.80	184.0
139.80	111.0
140.90	1144.0
141.90	208.0
142.90	1253.0
147.80	254.0
154.90	258.0
156.90	219.0
158.70	120.0
160.90	108.0
171.80	216.0
173.90	73728.0
175.00	5832.0
175.90	72080.0
176.90	5147.0
177.80	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
44.00	331.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42