




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052953.D
 Acq On : 03 Feb 2023 18:27
 Operator : JC/MD
 Sample : 01412-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M4

Manual IntegrationsAPPROVED

Quant Time: Feb 03 23:49:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 03 23:44:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/06/2023
 Supervised By :Mahesh Dadoda 02/06/2023

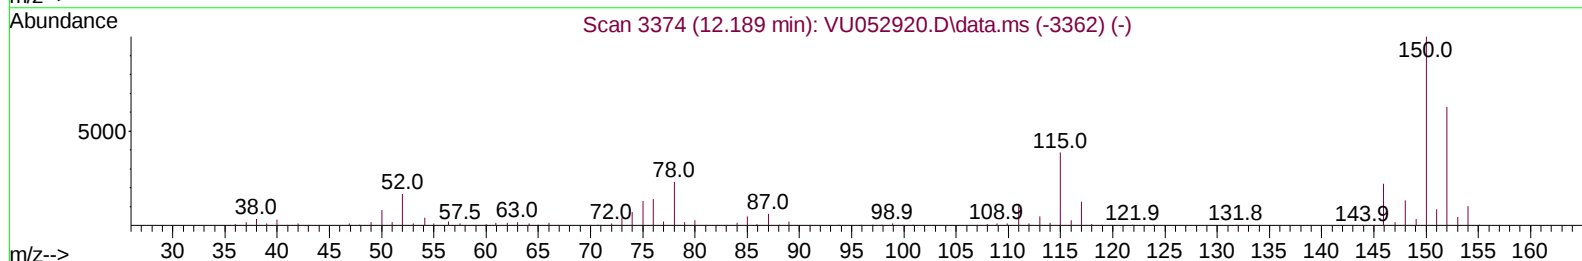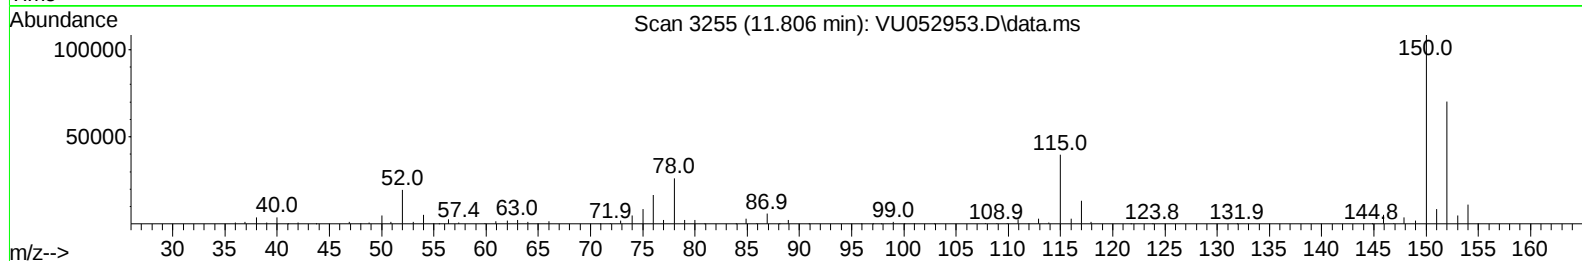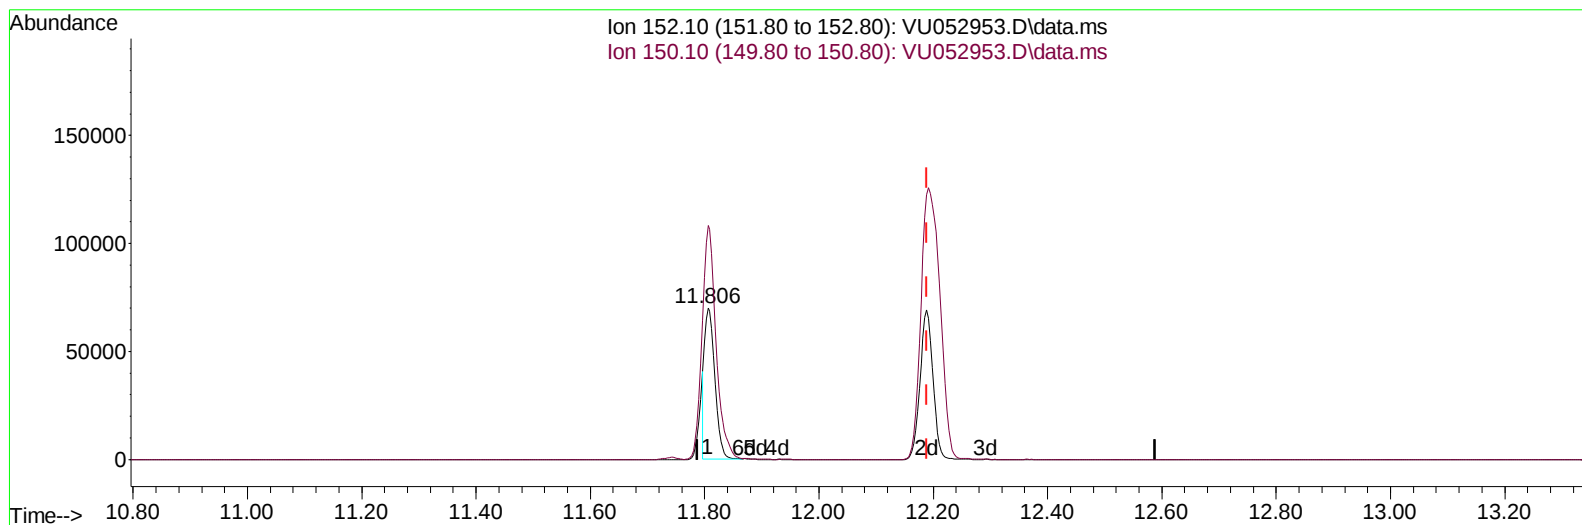

TIC: VU052953.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

11.806min (-0.382) 41.46 ug/L

response 87627

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	173.00	173.75
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052953.D
 Acq On : 03 Feb 2023 18:27
 Operator : JC/MD
 Sample : 01412-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M4

Manual IntegrationsAPPROVED

Quant Time: Feb 03 23:49:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 03 23:44:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/06/2023
 Supervised By :Mahesh Dadoda 02/06/2023

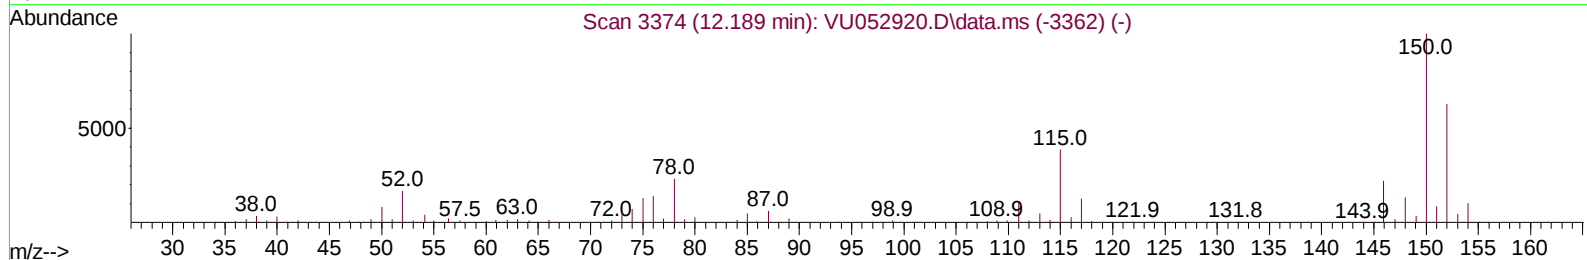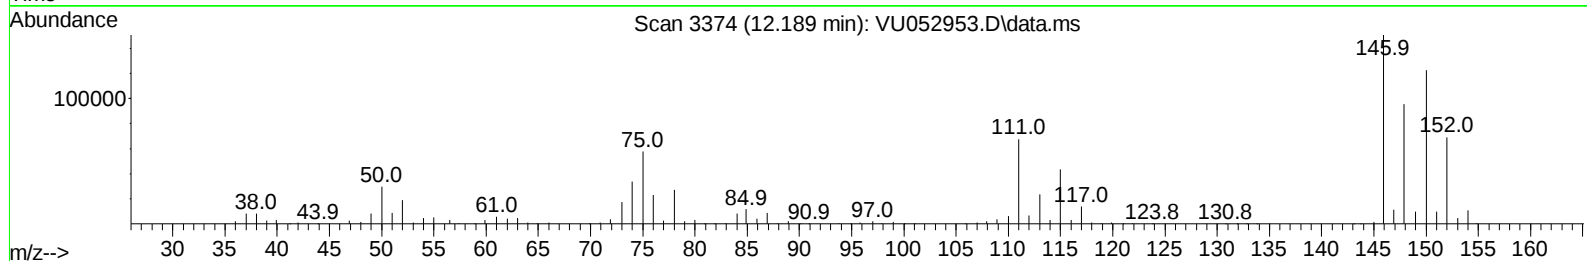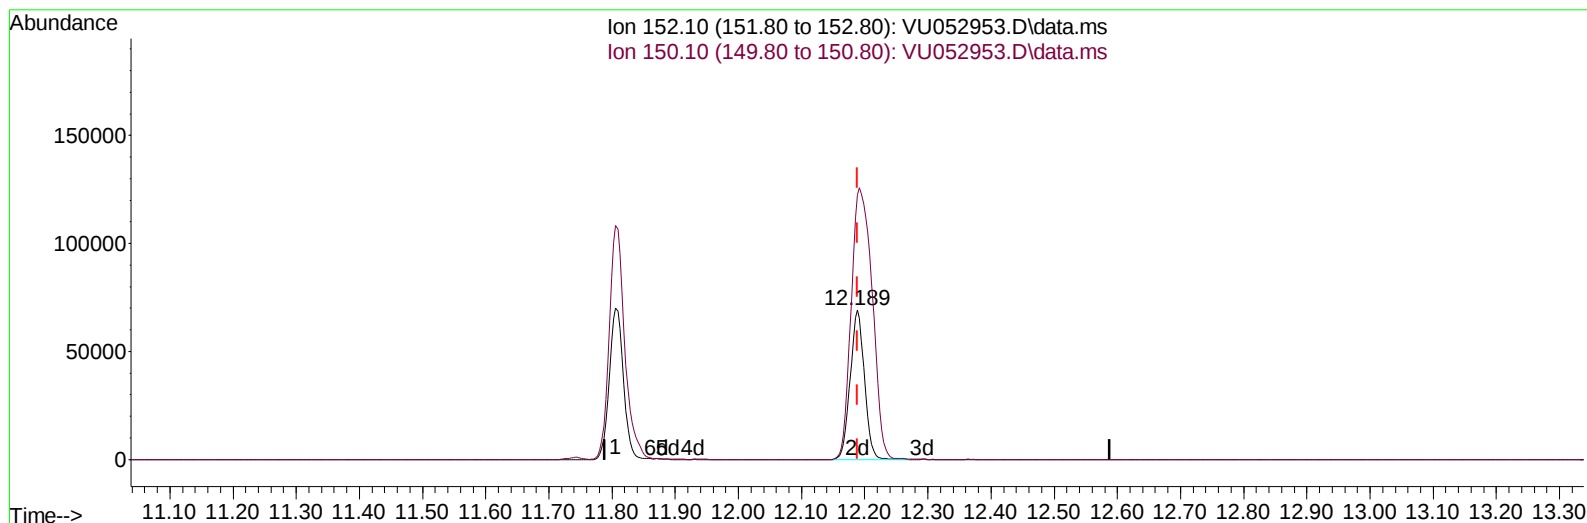

TIC: VU052953.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

12.189min (+ 0.000) 51.24 ug/L m

response 108285

Ion	Exp%	Act%
152.10	100.00	100.00
150.10	173.00	140.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052953.D
 Acq On : 03 Feb 2023 18:27
 Operator : JC/MD
 Sample : 01412-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M4

Manual IntegrationsAPPROVED

Quant Time: Feb 03 23:49:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 03 23:44:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/06/2023
 Supervised By :Mahesh Dadoda 02/06/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	204677	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	203937	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	108840	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56156	38.119	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	76.240%	
7) Chloroethane-d5	1.909	69	55975	46.113	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	92.220%	
11) 1,1-Dichloroethene-d2	2.565	63	91134	31.103	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	62.200%	
21) 2-Butanone-d5	4.616	46	70988	78.004	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	78.000%	
24) Chloroform-d	5.057	84	145664	46.331	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.660%	
26) 1,2-Dichloroethane-d4	5.697	65	96593	48.116	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.240%	
32) Benzene-d6	5.723	84	267274	42.897	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	85.800%	
36) 1,2-Dichloropropane-d6	6.684	67	80187	43.882	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	87.760%	
41) Toluene-d8	7.893	98	234381	41.311	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.620%	
43) trans-1,3-Dichloroprop...	8.176	79	39478	43.104	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	86.200%	
47) 2-Hexanone-d5	8.629	63	47474	73.939	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	73.940%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	114304	42.337	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	84.680%	
66) 1,2-Dichlorobenzene-d4	12.189	152	108285m	51.238	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	102.480%	
Target Compounds						
						Qvalue
20) cis-1,2-Dichloroethene	4.662	96	148074	84.758	ug/L	95
33) Benzene	5.771	78	6871	0.990	ug/L	100
34) Trichloroethene	6.539	95	16636	9.428	ug/L	96
51) Chlorobenzene	9.443	112	468406	95.693	ug/L	99
64) 1,3-Dichlorobenzene	11.742	146	14603	4.118	ug/L	97
65) 1,4-Dichlorobenzene	11.832	146	158387	43.139	ug/L	99
67) 1,2-Dichlorobenzene	12.208	146	1159974	323.363	ug/L	98
70) 1,2,4-trichlorobenzene	13.835	180	39603	17.991	ug/L	99
72) 1,2,3-Trichlorobenzene	14.323	180	7785	3.346	ug/L #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052953.D
Acq On : 03 Feb 2023 18:27
Operator : JC/MD
Sample : 01412-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M4

Manual IntegrationsAPPROVED

Quant Time: Feb 03 23:49:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 03 23:44:08 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 02/06/2023
Supervised By :Mahesh Dadoda 02/06/2023

