

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052942.D
 Acq On : 03 Feb 2023 14:00
 Operator : JC/MD
 Sample : 01381-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	99	rVB	77546	101482	3.12%	0.812%
2	1.906	169	176	194	rBV	68936	110650	3.41%	0.885%
3	2.163	254	256	259	rBV	539	323	0.01%	0.003%
4	2.559	364	379	397	rVB	171682	277737	8.55%	2.221%
5	2.633	398	402	403	rBV2	336	242	0.01%	0.002%
6	2.716	425	428	431	rBV	311	282	0.01%	0.002%
7	2.781	446	448	449	rBV	318	150	0.00%	0.001%
8	2.864	469	474	476	rBV2	229	204	0.01%	0.002%
9	2.896	482	484	487	rBV	227	174	0.01%	0.001%
10	2.945	496	499	502	rBV	152	153	0.00%	0.001%
11	3.041	518	529	544	rBB3	4229	8365	0.26%	0.067%
12	3.115	547	552	554	rBV	214	228	0.01%	0.002%
13	3.176	563	571	581	rVV3	959	2085	0.06%	0.017%
14	3.227	584	587	588	rBV3	284	159	0.00%	0.001%
15	3.350	615	625	638	rBB5	3368	6562	0.20%	0.052%
16	3.440	648	653	656	rBB	207	226	0.01%	0.002%
17	3.491	663	669	671	rBB	208	223	0.01%	0.002%
18	3.539	682	684	690	rBB2	319	288	0.01%	0.002%
19	3.813	767	769	772	rBB	260	142	0.00%	0.001%
20	3.854	777	782	784	rBV	315	299	0.01%	0.002%
21	3.945	808	810	813	rBV	172	136	0.00%	0.001%
22	3.977	816	820	822	rBV	270	172	0.01%	0.001%
23	4.044	839	841	846	rBV	235	217	0.01%	0.002%
24	4.157	872	876	879	rBB	264	247	0.01%	0.002%
25	4.330	926	930	932	rBB	171	143	0.00%	0.001%
26	4.658	1010	1032	1064	rBV2	406212	1015145	31.25%	8.119%
27	4.925	1113	1115	1118	rVV	193	140	0.00%	0.001%
28	5.057	1137	1156	1176	rBV	158464	351324	10.82%	2.810%
29	5.163	1187	1189	1192	rBV	320	237	0.01%	0.002%
30	5.237	1208	1212	1215	rBV	234	226	0.01%	0.002%
31	5.285	1223	1227	1231	rVB2	376	337	0.01%	0.003%
32	5.436	1273	1274	1278	rBV2	238	148	0.00%	0.001%
33	5.488	1284	1290	1292	rBB	159	181	0.01%	0.001%
34	5.719	1341	1362	1400	rBV2	307593	845402	26.03%	6.761%
35	6.141	1487	1493	1495	rBB	148	173	0.01%	0.001%
36	6.243	1512	1525	1544	rBV	255401	480868	14.81%	3.846%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052942.D
 Acq On : 03 Feb 2023 14:00
 Operator : JC/MD
 Sample : 01381-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.536	1602	1616	1634	rBV	358430	672620	20.71%	5.380%
38	6.684	1648	1662	1680	rBV	192317	371881	11.45%	2.974%
39	6.768	1686	1688	1690	rBV	253	152	0.00%	0.001%
40	6.877	1718	1722	1727	rBB	155	195	0.01%	0.002%
41	6.964	1747	1749	1754	rBB	148	151	0.00%	0.001%
42	7.079	1782	1785	1788	rVB	329	194	0.01%	0.002%
43	7.192	1813	1820	1823	rBV3	1565	1934	0.06%	0.015%
44	7.327	1859	1862	1869	rBB	212	241	0.01%	0.002%
45	7.362	1870	1873	1876	rBB	192	153	0.00%	0.001%
46	7.404	1883	1886	1889	rBB	165	136	0.00%	0.001%
47	7.562	1923	1935	1954	rBV	101023	175949	5.42%	1.407%
48	7.694	1965	1976	1980	rBV3	941	1342	0.04%	0.011%
49	7.739	1987	1990	1994	rBB	157	153	0.00%	0.001%
50	7.845	2019	2023	2025	rBV	145	150	0.00%	0.001%
51	7.893	2025	2038	2054	rBV	372931	636970	19.61%	5.094%
52	8.031	2079	2081	2084	rBV	522	327	0.01%	0.003%
53	8.176	2115	2126	2149	rBB	68240	122161	3.76%	0.977%
54	8.362	2182	2184	2187	rVB2	384	183	0.01%	0.001%
55	8.468	2208	2217	2226	rBB4	2323	3643	0.11%	0.029%
56	8.562	2243	2246	2250	rBV	223	228	0.01%	0.002%
57	8.649	2253	2273	2302	rBV3	138043	305584	9.41%	2.444%
58	8.812	2319	2324	2328	rBV	330	315	0.01%	0.003%
59	8.919	2348	2357	2359	rBV2	328	433	0.01%	0.003%
60	9.031	2389	2392	2396	rVB	311	192	0.01%	0.002%
61	9.099	2408	2413	2416	rBV	213	245	0.01%	0.002%
62	9.147	2424	2428	2431	rBB	260	186	0.01%	0.001%
63	9.166	2431	2434	2436	rBV	155	135	0.00%	0.001%
64	9.443	2499	2520	2543	rBV2	828338	1952446	60.11%	15.616%
65	9.629	2574	2578	2582	rBV2	394	344	0.01%	0.003%
66	9.645	2582	2583	2588	rVB	478	257	0.01%	0.002%
67	9.693	2593	2598	2602	rBV2	753	836	0.03%	0.007%
68	9.812	2632	2635	2638	rBB	205	162	0.00%	0.001%
69	9.989	2681	2690	2692	rBV	176	327	0.01%	0.003%
70	10.099	2721	2724	2730	rVB2	670	567	0.02%	0.005%
71	10.218	2758	2761	2763	rBV	284	182	0.01%	0.001%
72	10.385	2810	2813	2815	rBB	246	142	0.00%	0.001%
73	10.410	2816	2821	2824	rBV	218	286	0.01%	0.002%
74	10.529	2855	2858	2861	rBV	172	162	0.00%	0.001%
75	10.758	2917	2929	2945	rBV	258119	415466	12.79%	3.323%
76	10.854	2956	2959	2962	rBV2	708	529	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052942.D
 Acq On : 03 Feb 2023 14:00
 Operator : JC/MD
 Sample : 01381-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.886	2962	2969	2980	rVB4	2687	4208	0.13%	0.034%
78	10.986	2996	3000	3008	rVB2	1229	1057	0.03%	0.008%
79	11.041	3014	3017	3020	rBV	157	153	0.00%	0.001%
80	11.124	3040	3043	3046	rBV	210	179	0.01%	0.001%
81	11.295	3089	3096	3104	rBB	632	925	0.03%	0.007%
82	11.404	3127	3130	3132	rBV	194	163	0.01%	0.001%
83	11.465	3145	3149	3153	rBV2	427	375	0.01%	0.003%
84	11.645	3202	3205	3208	rBV	206	191	0.01%	0.002%
85	11.742	3225	3235	3245	rBV2	36740	57201	1.76%	0.457%
86	11.812	3245	3257	3281	rVB2	407622	1044311	32.15%	8.352%
87	11.954	3296	3301	3304	rBV	312	285	0.01%	0.002%
88	12.012	3317	3319	3323	rBV	319	239	0.01%	0.002%
89	12.066	3331	3336	3339	rBV3	966	966	0.03%	0.008%
90	12.208	3362	3380	3403	rBV2	1763730	3247969	100.00%	25.977%
91	12.401	3437	3440	3444	rBV2	290	220	0.01%	0.002%
92	12.587	3495	3498	3501	rBV	242	223	0.01%	0.002%
93	13.224	3690	3696	3700	rVB4	882	845	0.03%	0.007%
94	13.587	3806	3809	3812	rVB	277	151	0.00%	0.001%
95	13.754	3859	3861	3865	rBV	263	190	0.01%	0.002%
96	13.835	3873	3886	3901	rBV	145162	231839	7.14%	1.854%
97	14.205	3996	4001	4003	rBV2	309	254	0.01%	0.002%
98	14.279	4020	4024	4025	rBV	235	181	0.01%	0.001%
99	14.327	4030	4039	4051	rVV3	24455	38137	1.17%	0.305%
100	14.520	4095	4099	4103	rBV2	306	313	0.01%	0.003%




Sum of corrected areas: 12503204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052942.D
Acq On : 03 Feb 2023 14:00
Operator : JC/MD
Sample : 01381-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

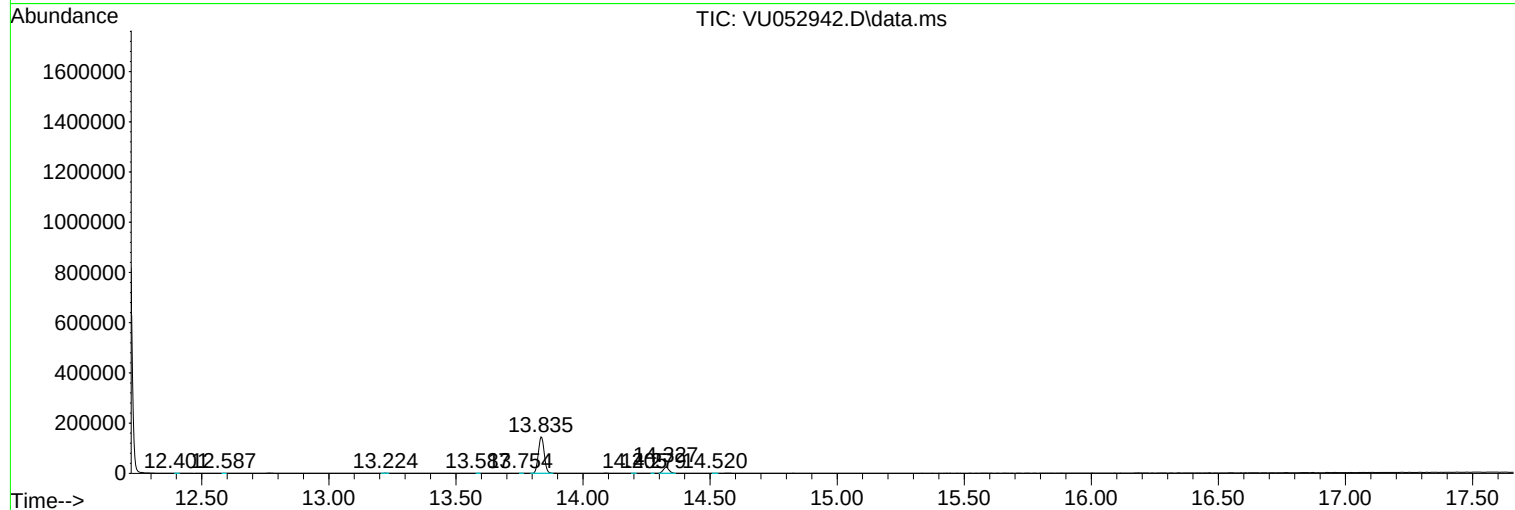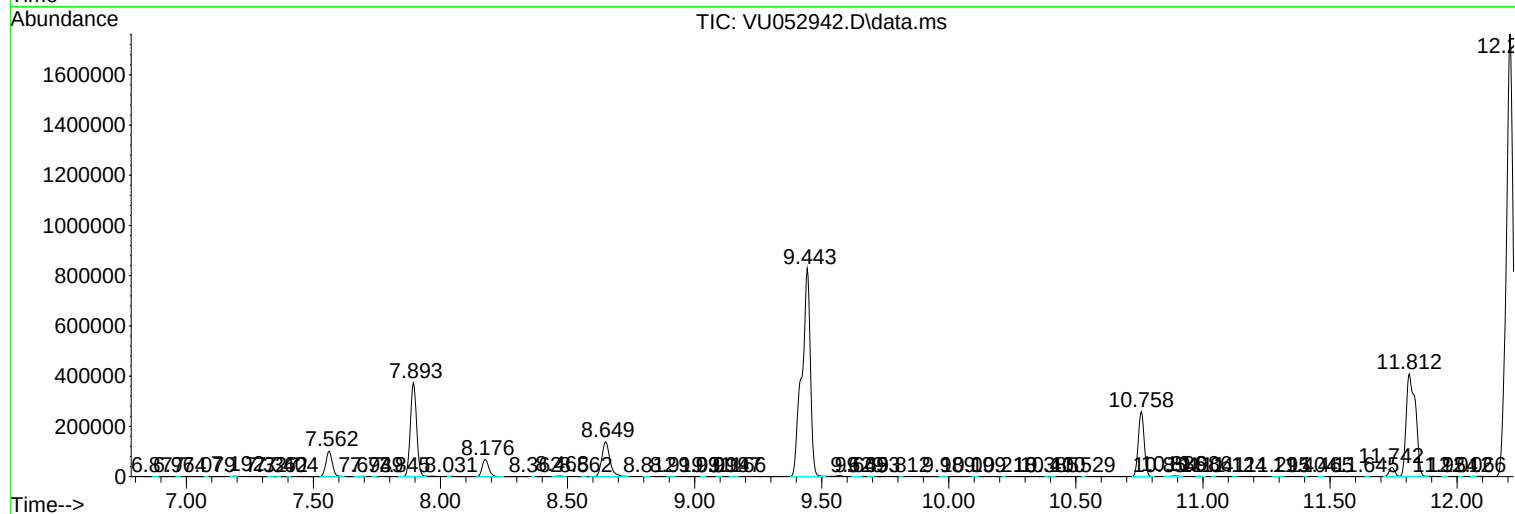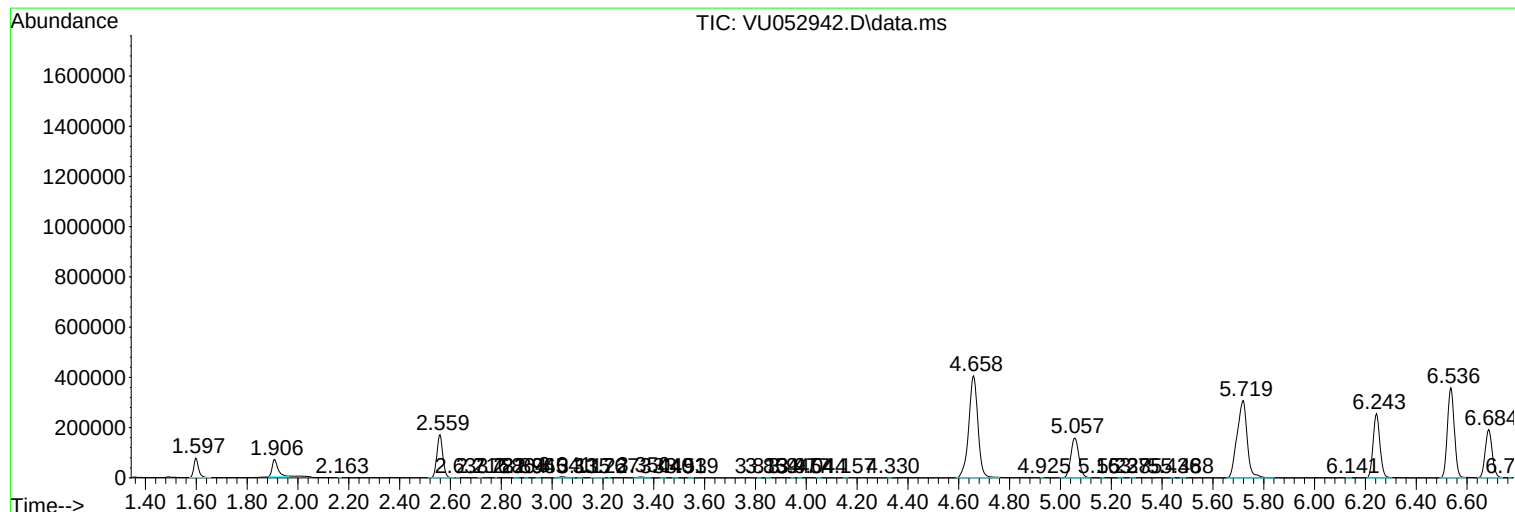

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052942.D
Acq On : 03 Feb 2023 14:00
Operator : JC/MD
Sample : 01381-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052942.D
Acq On : 03 Feb 2023 14:00
Operator : JC/MD
Sample : 01381-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44N3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc