

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052946.D
 Acq On : 03 Feb 2023 15:39
 Operator : JC/MD
 Sample : 01381-25 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	98	rVB	78659	99774	11.74%	1.630%
2	2.559	367	379	397	rBV	172537	281347	33.09%	4.597%
3	2.719	425	429	433	rBV2	531	629	0.07%	0.010%
4	2.780	445	448	450	rBV	329	251	0.03%	0.004%
5	2.938	493	497	499	rBB	170	111	0.01%	0.002%
6	3.041	517	529	544	rBV3	8490	17371	2.04%	0.284%
7	3.179	559	572	579	rBV3	1810	3615	0.43%	0.059%
8	3.250	591	594	598	rBV2	306	271	0.03%	0.004%
9	3.330	617	619	622	rBV	266	109	0.01%	0.002%
10	3.378	629	634	638	rBB	173	185	0.02%	0.003%
11	3.417	644	646	649	rBV	137	116	0.01%	0.002%
12	3.517	673	677	680	rBB	178	172	0.02%	0.003%
13	3.539	681	684	686	rBV	131	112	0.01%	0.002%
14	3.652	715	719	721	rBV	143	119	0.01%	0.002%
15	3.703	732	735	739	rBV	240	235	0.03%	0.004%
16	3.832	773	775	780	rBB	145	118	0.01%	0.002%
17	3.944	806	810	812	rBV	203	148	0.02%	0.002%
18	4.147	871	873	878	rBB	284	207	0.02%	0.003%
19	4.253	903	906	908	rBB	165	111	0.01%	0.002%
20	4.288	912	917	919	rBB2	275	240	0.03%	0.004%
21	4.314	923	925	928	rBB	187	121	0.01%	0.002%
22	4.362	938	940	942	rBV	169	111	0.01%	0.002%
23	4.430	958	961	963	rBV	184	144	0.02%	0.002%
24	4.520	985	989	991	rBB	284	185	0.02%	0.003%
25	4.549	995	998	1002	rBB	209	178	0.02%	0.003%
26	4.626	1009	1022	1054	rBV2	47927	138401	16.28%	2.261%
27	4.870	1096	1098	1101	rBV2	306	207	0.02%	0.003%
28	5.057	1138	1156	1179	rBV	163677	361435	42.51%	5.905%
29	5.250	1213	1216	1217	rBV	284	166	0.02%	0.003%
30	5.414	1264	1267	1271	rBB	172	177	0.02%	0.003%
31	5.462	1279	1282	1287	rBV	171	214	0.03%	0.003%
32	5.533	1301	1304	1307	rBB	142	124	0.01%	0.002%
33	5.597	1322	1324	1327	rBB	168	105	0.01%	0.002%
34	5.719	1340	1362	1382	rBV2	314065	850214	100.00%	13.892%
35	5.886	1411	1414	1417	rBV	281	242	0.03%	0.004%
36	6.060	1464	1468	1472	rBB	166	171	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052946.D
 Acq On : 03 Feb 2023 15:39
 Operator : JC/MD
 Sample : 01381-25 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.099	1478	1480	1483	rBB	159	105	0.01%	0.002%
38	6.153	1493	1497	1499	rBB	182	113	0.01%	0.002%
39	6.243	1511	1525	1544	rBV	250620	469866	55.26%	7.677%
40	6.504	1603	1606	1607	rBV	200	132	0.02%	0.002%
41	6.684	1649	1662	1680	rBV	195297	381918	44.92%	6.240%
42	6.784	1692	1693	1695	rBV	232	113	0.01%	0.002%
43	6.796	1695	1697	1699	rVV	304	178	0.02%	0.003%
44	7.076	1781	1784	1787	rBB2	363	246	0.03%	0.004%
45	7.185	1812	1818	1829	rBV4	1224	2108	0.25%	0.034%
46	7.359	1868	1872	1875	rBB	191	179	0.02%	0.003%
47	7.507	1916	1918	1922	rBV	150	152	0.02%	0.002%
48	7.562	1923	1935	1953	rVV	103670	181081	21.30%	2.959%
49	7.755	1993	1995	1998	rBB	257	117	0.01%	0.002%
50	7.787	2002	2005	2009	rBB	173	168	0.02%	0.003%
51	7.893	2025	2038	2058	rBV	384226	654239	76.95%	10.690%
52	8.176	2114	2126	2139	rBV	73968	123972	14.58%	2.026%
53	8.311	2166	2168	2170	rBV	180	119	0.01%	0.002%
54	8.346	2174	2179	2182	rBB	234	238	0.03%	0.004%
55	8.369	2183	2186	2188	rBV	234	152	0.02%	0.002%
56	8.427	2201	2204	2207	rBB	179	141	0.02%	0.002%
57	8.472	2213	2218	2221	rBB2	297	272	0.03%	0.004%
58	8.507	2226	2229	2234	rBV	123	175	0.02%	0.003%
59	8.642	2258	2271	2307	rBV2	144385	312404	36.74%	5.104%
60	8.870	2336	2342	2345	rBV2	480	493	0.06%	0.008%
61	8.931	2358	2361	2364	rBV	142	143	0.02%	0.002%
62	9.002	2381	2383	2385	rBV	164	108	0.01%	0.002%
63	9.057	2397	2400	2407	rBB	239	292	0.03%	0.005%
64	9.153	2427	2430	2434	rBV2	261	240	0.03%	0.004%
65	9.195	2440	2443	2447	rBV	122	131	0.02%	0.002%
66	9.343	2486	2489	2491	rBV	156	129	0.02%	0.002%
67	9.414	2498	2511	2531	rBV	348174	585610	68.88%	9.568%
68	9.687	2590	2596	2598	rBV	223	263	0.03%	0.004%
69	9.918	2664	2668	2670	rBB	128	109	0.01%	0.002%
70	9.934	2670	2673	2676	rBV	239	195	0.02%	0.003%
71	9.970	2680	2684	2687	rBB	159	152	0.02%	0.002%
72	10.108	2724	2727	2730	rBV	150	162	0.02%	0.003%
73	10.211	2756	2759	2762	rBB	286	202	0.02%	0.003%
74	10.234	2762	2766	2767	rBV	231	163	0.02%	0.003%
75	10.282	2776	2781	2784	rBV	342	309	0.04%	0.005%
76	10.378	2808	2811	2812	rBV	167	113	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052946.D
 Acq On : 03 Feb 2023 15:39
 Operator : JC/MD
 Sample : 01381-25 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.420	2820	2824	2825	rBV	357	163	0.02%	0.003%
78	10.471	2835	2840	2841	rBV	236	187	0.02%	0.003%
79	10.507	2847	2851	2855	rBB	200	176	0.02%	0.003%
80	10.529	2855	2858	2864	rBV	215	273	0.03%	0.004%
81	10.616	2881	2885	2886	rBV	145	121	0.01%	0.002%
82	10.754	2916	2928	2947	rVB	272047	429715	50.54%	7.021%
83	10.848	2954	2957	2962	rBB	128	113	0.01%	0.002%
84	10.893	2963	2971	2975	rBB2	290	417	0.05%	0.007%
85	10.922	2975	2980	2984	rBV	185	258	0.03%	0.004%
86	11.031	3011	3014	3020	rBB	192	200	0.02%	0.003%
87	11.066	3021	3025	3028	rBV	325	280	0.03%	0.005%
88	11.320	3099	3104	3107	rBV	191	230	0.03%	0.004%
89	11.439	3139	3141	3143	rBV	175	117	0.01%	0.002%
90	11.468	3148	3150	3152	rBV	178	124	0.01%	0.002%
91	11.809	3244	3256	3278	rBV	361831	569091	66.94%	9.298%
92	12.076	3335	3339	3343	rBV	315	358	0.04%	0.006%
93	12.188	3362	3374	3398	rBV	386380	641626	75.47%	10.484%
94	12.626	3505	3510	3512	rBV	363	309	0.04%	0.005%
95	12.658	3517	3520	3522	rBV	223	183	0.02%	0.003%
96	12.770	3547	3555	3560	rBV2	890	1254	0.15%	0.020%
97	12.838	3573	3576	3581	rBB	216	232	0.03%	0.004%
98	12.928	3602	3604	3605	rBV	313	154	0.02%	0.003%
99	13.391	3745	3748	3749	rBV	226	156	0.02%	0.003%
100	14.230	4005	4009	4010	rBV2	240	160	0.02%	0.003%




Sum of corrected areas: 6120335

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052946.D
Acq On : 03 Feb 2023 15:39
Operator : JC/MD
Sample : 01381-25 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

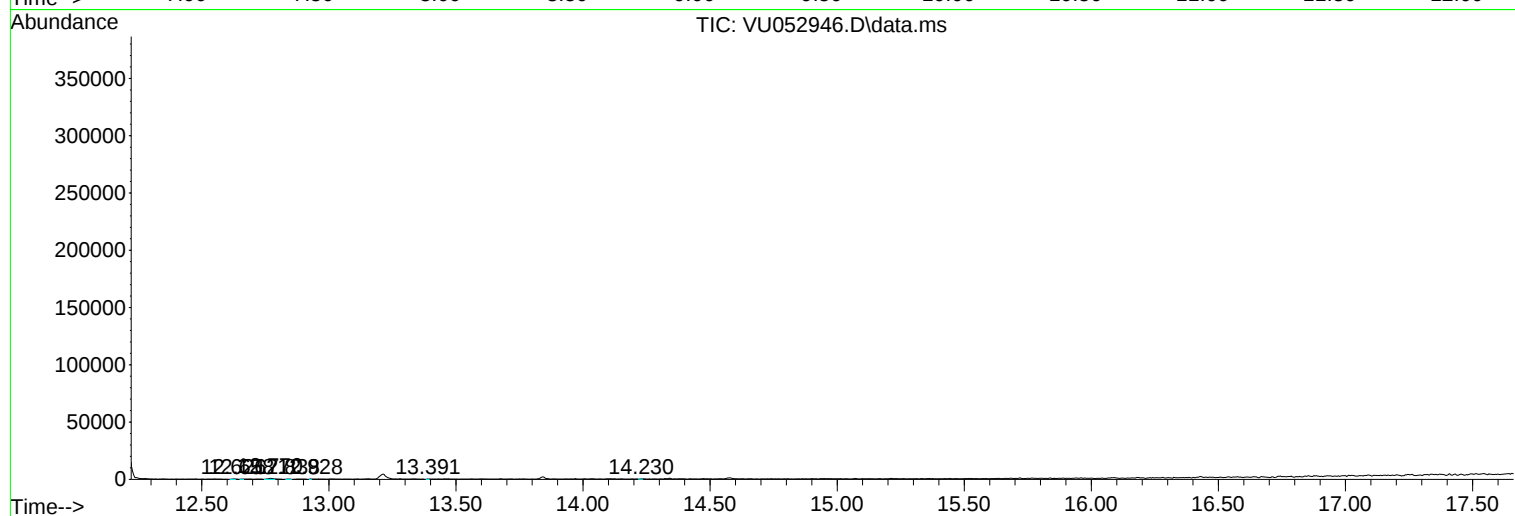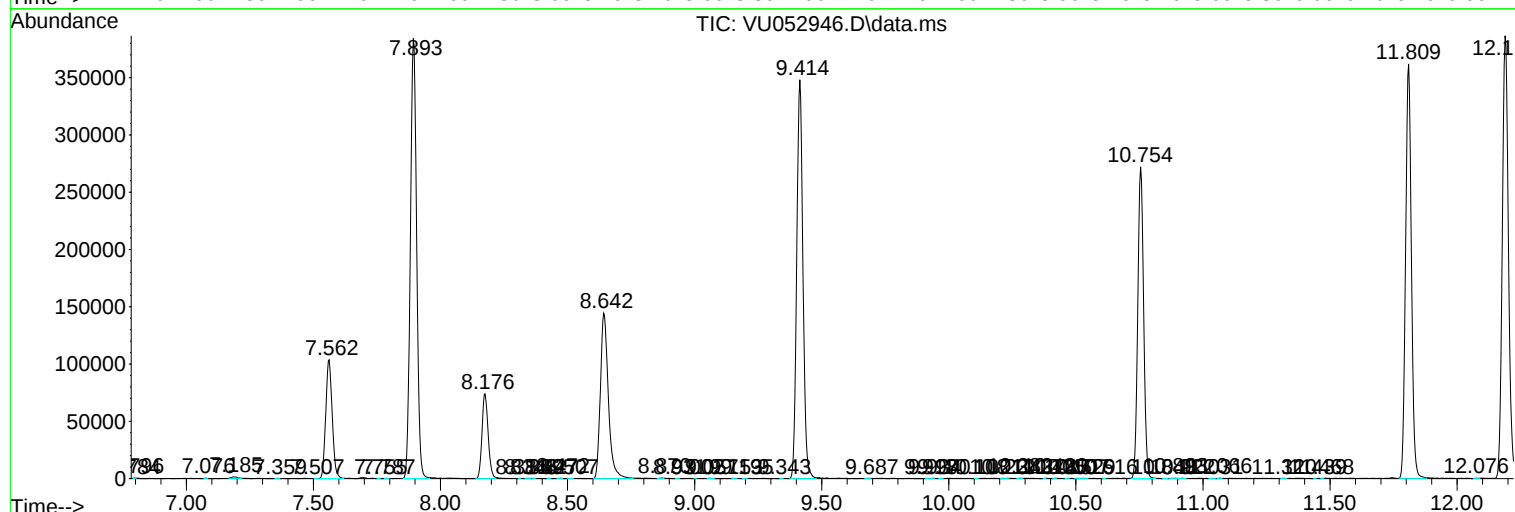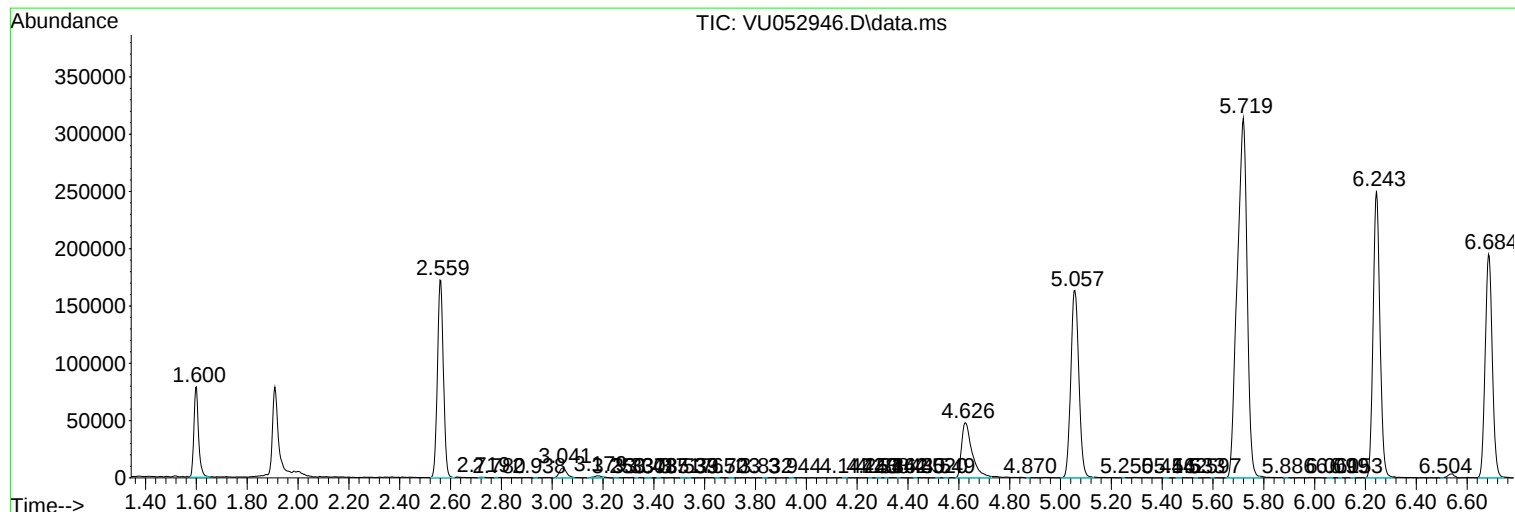

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052946.D
Acq On : 03 Feb 2023 15:39
Operator : JC/MD
Sample : 01381-25 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052946.D
Acq On : 03 Feb 2023 15:39
Operator : JC/MD
Sample : 01381-25 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc