

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052947.D
 Acq On : 03 Feb 2023 16:02
 Operator : JC/MD
 Sample : 01412-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	101	rVB	73773	94535	10.79%	1.474%
2	2.559	367	379	397	rBV	169032	272049	31.06%	4.241%
3	2.694	416	421	424	rBV	257	276	0.03%	0.004%
4	2.784	445	449	454	rBV	424	583	0.07%	0.009%
5	2.890	477	482	486	rBB	168	184	0.02%	0.003%
6	2.986	509	512	515	rBB	214	158	0.02%	0.002%
7	3.041	516	529	539	rBV4	4037	7993	0.91%	0.125%
8	3.179	562	572	576	rBV2	681	1180	0.13%	0.018%
9	3.237	586	590	593	rBB	158	127	0.01%	0.002%
10	3.285	599	605	608	rBB	191	234	0.03%	0.004%
11	3.555	686	689	692	rBV	199	188	0.02%	0.003%
12	3.642	713	716	719	rBB	163	132	0.02%	0.002%
13	3.848	777	780	781	rBV	235	124	0.01%	0.002%
14	4.060	843	846	849	rBB2	283	183	0.02%	0.003%
15	4.089	850	855	857	rBV	172	155	0.02%	0.002%
16	4.166	876	879	882	rBB	141	119	0.01%	0.002%
17	4.250	901	905	907	rBB	146	124	0.01%	0.002%
18	4.288	912	917	920	rBV	146	165	0.02%	0.003%
19	4.375	942	944	949	rBB	179	166	0.02%	0.003%
20	4.501	981	983	985	rBV	169	110	0.01%	0.002%
21	4.626	1010	1022	1052	rBV	47398	135707	15.49%	2.116%
22	4.893	1100	1105	1107	rBV2	235	202	0.02%	0.003%
23	4.951	1119	1123	1127	rBV	154	207	0.02%	0.003%
24	5.005	1136	1140	1141	rBV	245	170	0.02%	0.003%
25	5.057	1141	1156	1175	rVV	158882	346473	39.56%	5.401%
26	5.185	1192	1196	1199	rBV	175	208	0.02%	0.003%
27	5.224	1206	1208	1212	rBV	120	129	0.01%	0.002%
28	5.411	1262	1266	1268	rBB	152	124	0.01%	0.002%
29	5.462	1279	1282	1287	rBB	209	199	0.02%	0.003%
30	5.584	1317	1320	1323	rBB	154	126	0.01%	0.002%
31	5.719	1341	1362	1384	rBV2	301582	817353	93.31%	12.742%
32	5.912	1418	1422	1424	rBB	280	154	0.02%	0.002%
33	5.938	1427	1430	1432	rBV	175	142	0.02%	0.002%
34	5.999	1446	1449	1452	rBB	208	154	0.02%	0.002%
35	6.195	1508	1510	1512	rBV	172	107	0.01%	0.002%
36	6.243	1512	1525	1543	rVV2	256506	479731	54.77%	7.479%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052947.D
 Acq On : 03 Feb 2023 16:02
 Operator : JC/MD
 Sample : 01412-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.439	1581	1586	1590	rBB	261	291	0.03%	0.005%
38	6.536	1605	1616	1632	rBV3	26880	50145	5.72%	0.782%
39	6.684	1649	1662	1682	rVV	190587	369847	42.22%	5.766%
40	6.806	1694	1700	1703	rBB3	402	381	0.04%	0.006%
41	6.851	1710	1714	1717	rBV	157	189	0.02%	0.003%
42	6.951	1743	1745	1749	rBB	134	110	0.01%	0.002%
43	7.121	1793	1798	1801	rBB	241	233	0.03%	0.004%
44	7.185	1811	1818	1828	rBV6	1524	2698	0.31%	0.042%
45	7.465	1902	1905	1909	rBB	122	111	0.01%	0.002%
46	7.497	1910	1915	1918	rBB	138	164	0.02%	0.003%
47	7.558	1919	1934	1953	rBV	97932	173586	19.82%	2.706%
48	7.780	1999	2003	2005	rBB	138	117	0.01%	0.002%
49	7.838	2018	2021	2024	rBB	156	131	0.01%	0.002%
50	7.893	2025	2038	2059	rBV	367406	630101	71.94%	9.823%
51	8.108	2102	2105	2109	rBV	211	206	0.02%	0.003%
52	8.176	2114	2126	2142	rBV2	70425	120350	13.74%	1.876%
53	8.362	2180	2184	2187	rBB	160	161	0.02%	0.003%
54	8.426	2201	2204	2207	rBV	148	152	0.02%	0.002%
55	8.645	2259	2272	2304	rBV3	141943	310999	35.51%	4.848%
56	8.822	2325	2327	2330	rVB	290	105	0.01%	0.002%
57	8.880	2342	2345	2347	rBV	165	133	0.02%	0.002%
58	8.909	2351	2354	2356	rBV	247	139	0.02%	0.002%
59	8.963	2368	2371	2376	rBV	225	224	0.03%	0.003%
60	9.012	2381	2386	2389	rBB	236	236	0.03%	0.004%
61	9.057	2398	2400	2403	rBV	141	124	0.01%	0.002%
62	9.163	2429	2433	2435	rBV	261	212	0.02%	0.003%
63	9.234	2453	2455	2459	rBB	165	109	0.01%	0.002%
64	9.288	2468	2472	2474	rBV	176	143	0.02%	0.002%
65	9.414	2498	2511	2535	rBV	358844	653638	74.62%	10.190%
66	9.613	2569	2573	2576	rBV	195	213	0.02%	0.003%
67	9.658	2584	2587	2591	rBB	190	174	0.02%	0.003%
68	9.703	2599	2601	2603	rBV	181	115	0.01%	0.002%
69	9.799	2628	2631	2635	rBV	196	202	0.02%	0.003%
70	9.838	2639	2643	2645	rBV	261	258	0.03%	0.004%
71	9.883	2654	2657	2663	rBV	191	244	0.03%	0.004%
72	10.063	2709	2713	2715	rBB	154	126	0.01%	0.002%
73	10.140	2734	2737	2739	rBV	192	142	0.02%	0.002%
74	10.182	2746	2750	2753	rBB	144	118	0.01%	0.002%
75	10.250	2768	2771	2773	rBB	312	169	0.02%	0.003%
76	10.330	2793	2796	2799	rBB	267	185	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052947.D
 Acq On : 03 Feb 2023 16:02
 Operator : JC/MD
 Sample : 01412-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44M3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.352	2799	2803	2805	rBB	233	176	0.02%	0.003%
78	10.388	2812	2814	2816	rBV	170	114	0.01%	0.002%
79	10.430	2822	2827	2831	rBB	146	148	0.02%	0.002%
80	10.452	2832	2834	2837	rBB	177	116	0.01%	0.002%
81	10.475	2838	2841	2843	rBV	208	150	0.02%	0.002%
82	10.507	2847	2851	2852	rBV	223	141	0.02%	0.002%
83	10.584	2865	2875	2877	rBV	216	384	0.04%	0.006%
84	10.626	2886	2888	2890	rBV	151	103	0.01%	0.002%
85	10.754	2917	2928	2946	rVB	259908	418004	47.72%	6.517%
86	10.844	2952	2956	2959	rBV	188	188	0.02%	0.003%
87	10.989	2998	3001	3004	rBB	198	153	0.02%	0.002%
88	11.008	3004	3007	3009	rBV	186	156	0.02%	0.002%
89	11.082	3028	3030	3033	rBV	157	126	0.01%	0.002%
90	11.156	3048	3053	3056	rBV	410	360	0.04%	0.006%
91	11.275	3087	3090	3094	rBB	182	164	0.02%	0.003%
92	11.301	3094	3098	3102	rBB	234	261	0.03%	0.004%
93	11.677	3212	3215	3217	rBV	177	149	0.02%	0.002%
94	11.745	3227	3236	3244	rBV2	7339	10645	1.22%	0.166%
95	11.809	3244	3256	3277	rVV	371646	628179	71.72%	9.793%
96	11.992	3310	3313	3315	rBV	148	126	0.01%	0.002%
97	12.192	3362	3375	3402	rBV2	420802	875912	100.00%	13.655%
98	12.330	3416	3418	3422	rBV2	386	281	0.03%	0.004%
99	13.593	3805	3811	3815	rBV	369	427	0.05%	0.007%
100	14.323	4035	4038	4047	rVB2	796	1052	0.12%	0.016%




Sum of corrected areas: 6414467

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052947.D
Acq On : 03 Feb 2023 16:02
Operator : JC/MD
Sample : 01412-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

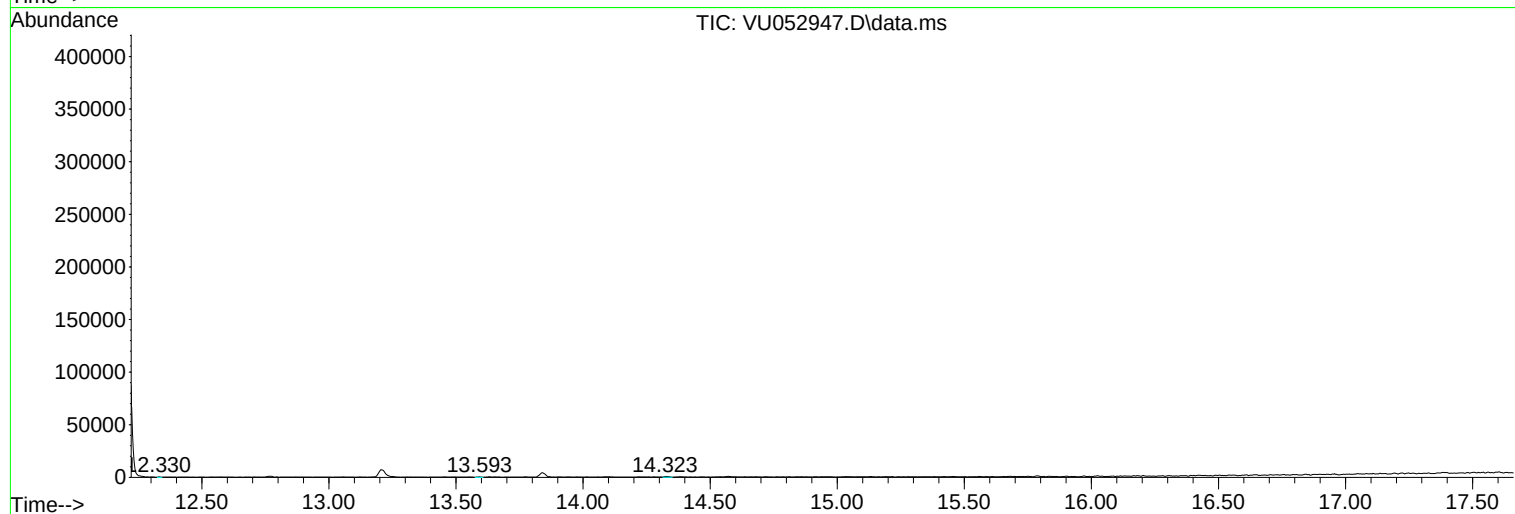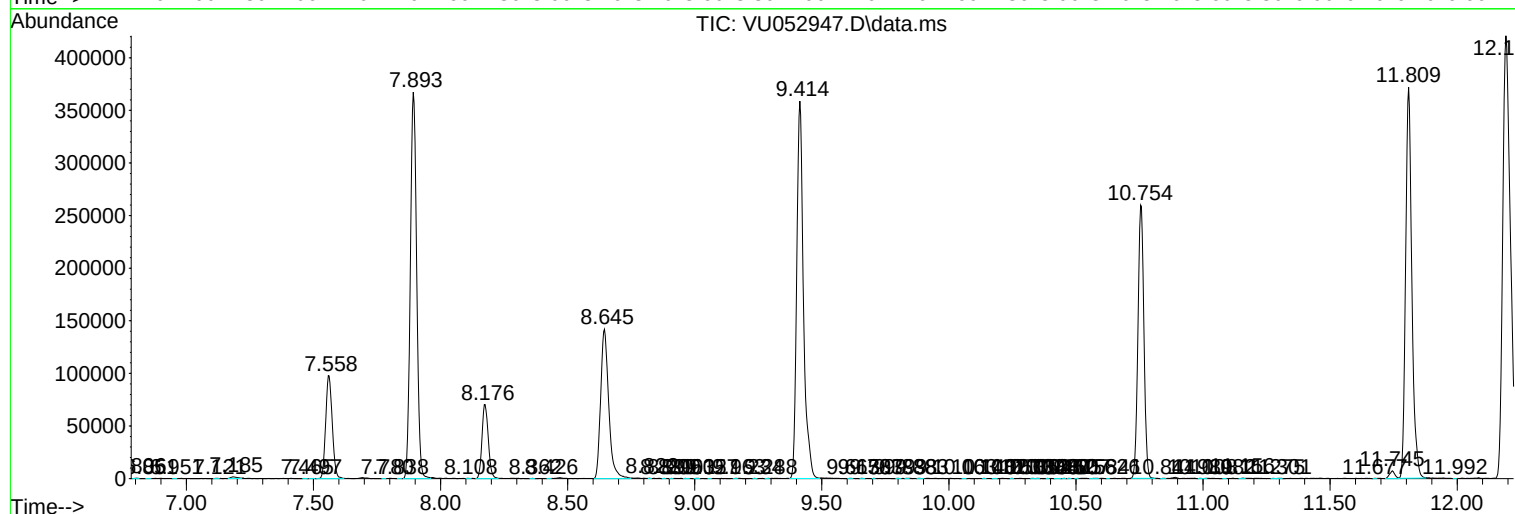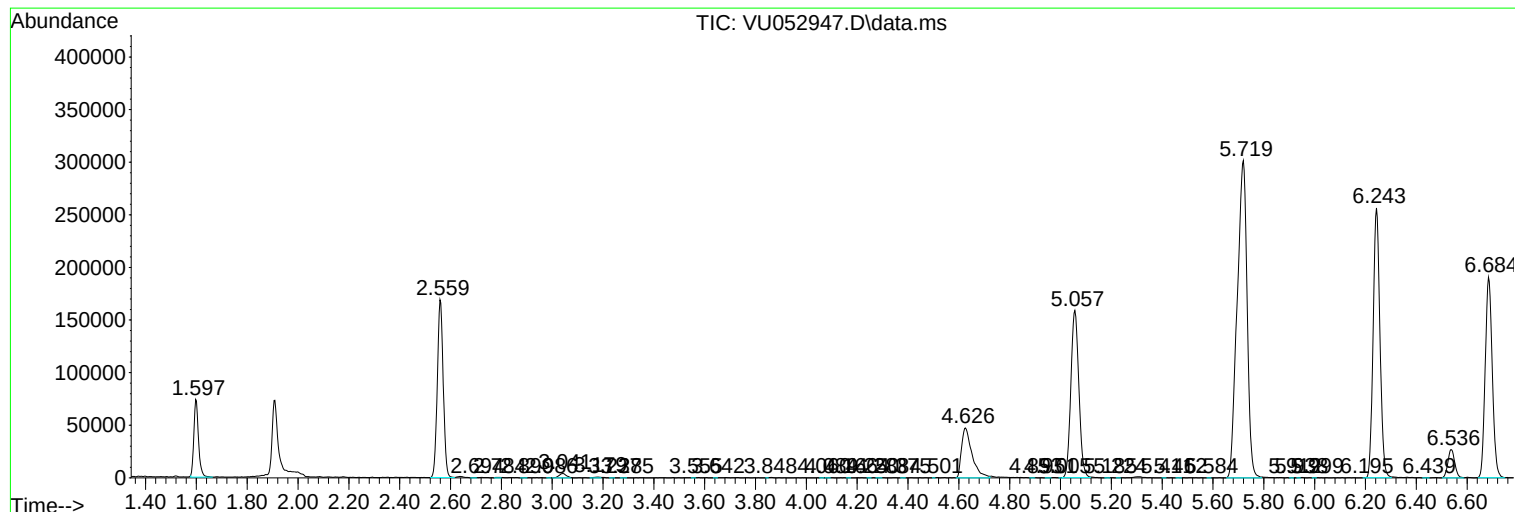

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052947.D
Acq On : 03 Feb 2023 16:02
Operator : JC/MD
Sample : 01412-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052947.D
Acq On : 03 Feb 2023 16:02
Operator : JC/MD
Sample : 01412-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc