

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052951.D
 Acq On : 03 Feb 2023 17:40
 Operator : JC/MD
 Sample : 01381-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	69254	82208	10.43%	1.430%
2	1.909	169	177	197	rVB	74449	102221	12.97%	1.779%
3	2.240	278	280	283	rBV	324	221	0.03%	0.004%
4	2.488	355	357	364	rVB	190	157	0.02%	0.003%
5	2.565	369	381	398	rVV	146090	235610	29.91%	4.100%
6	2.636	401	403	407	rVB2	311	159	0.02%	0.003%
7	2.687	416	419	422	rBV	209	190	0.02%	0.003%
8	3.041	520	529	543	rVB3	7175	13593	1.73%	0.237%
9	3.128	553	556	558	rBB	268	130	0.02%	0.002%
10	3.173	559	570	571	rBV	1812	1753	0.22%	0.031%
11	3.414	643	645	647	rVB	249	135	0.02%	0.002%
12	3.436	651	652	656	rBB	255	133	0.02%	0.002%
13	3.481	664	666	670	rBV	152	146	0.02%	0.003%
14	3.533	679	682	686	rBB	230	190	0.02%	0.003%
15	3.600	700	703	709	rBV	166	247	0.03%	0.004%
16	4.009	826	830	834	rBB2	246	199	0.03%	0.003%
17	4.620	1009	1020	1059	rBV	55099	144339	18.32%	2.512%
18	4.832	1084	1086	1092	rVB2	347	340	0.04%	0.006%
19	4.874	1097	1099	1103	rBV	239	158	0.02%	0.003%
20	4.932	1113	1117	1120	rBB2	266	194	0.02%	0.003%
21	5.057	1140	1156	1179	rBV	152136	333921	42.38%	5.810%
22	5.256	1214	1218	1221	rBV	197	203	0.03%	0.004%
23	5.719	1341	1362	1383	rVV3	287670	787844	100.00%	13.709%
24	5.886	1412	1414	1418	rBB	255	190	0.02%	0.003%
25	6.038	1457	1461	1462	rBV	231	187	0.02%	0.003%
26	6.083	1472	1475	1478	rBB	175	137	0.02%	0.002%
27	6.124	1485	1488	1491	rBB	203	148	0.02%	0.003%
28	6.243	1511	1525	1543	rBV	228017	422526	53.63%	7.352%
29	6.346	1553	1557	1559	rBV	297	168	0.02%	0.003%
30	6.530	1609	1614	1615	rBV2	1444	1194	0.15%	0.021%
31	6.684	1648	1662	1682	rBV	186361	356633	45.27%	6.205%
32	6.755	1682	1684	1687	rVB2	554	267	0.03%	0.005%
33	6.780	1688	1692	1694	rBB	249	139	0.02%	0.002%
34	6.800	1694	1698	1699	rBV	295	207	0.03%	0.004%
35	6.806	1699	1700	1705	rVB2	496	266	0.03%	0.005%
36	6.838	1706	1710	1712	rBB	159	129	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052951.D
 Acq On : 03 Feb 2023 17:40
 Operator : JC/MD
 Sample : 01381-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.854	1713	1715	1720	rBV	306	231	0.03%	0.004%
38	6.906	1727	1731	1735	rBV	260	247	0.03%	0.004%
39	6.948	1741	1744	1747	rBV	139	144	0.02%	0.003%
40	7.137	1800	1803	1806	rBB	162	131	0.02%	0.002%
41	7.185	1811	1818	1827	rBV4	1627	2399	0.30%	0.042%
42	7.221	1827	1829	1833	rVB2	273	180	0.02%	0.003%
43	7.558	1923	1934	1951	rVV	94072	166992	21.20%	2.906%
44	7.616	1951	1952	1955	rVB2	369	137	0.02%	0.002%
45	7.681	1968	1972	1973	rBV	633	465	0.06%	0.008%
46	7.893	2022	2038	2059	rBV	344664	596970	75.77%	10.387%
47	8.060	2086	2090	2092	rVB	293	221	0.03%	0.004%
48	8.083	2094	2097	2100	rVB2	373	208	0.03%	0.004%
49	8.176	2113	2126	2144	rBV	69314	116871	14.83%	2.034%
50	8.279	2154	2158	2162	rBB	430	292	0.04%	0.005%
51	8.449	2206	2211	2212	rBV	201	175	0.02%	0.003%
52	8.462	2212	2215	2218	rVB	280	211	0.03%	0.004%
53	8.591	2250	2255	2256	rBV	183	179	0.02%	0.003%
54	8.629	2256	2267	2296	rVV2	157103	304782	38.69%	5.303%
55	8.915	2352	2356	2359	rBV	154	179	0.02%	0.003%
56	8.964	2368	2371	2375	rBV	186	197	0.03%	0.003%
57	9.025	2387	2390	2393	rBV	199	187	0.02%	0.003%
58	9.201	2443	2445	2449	rBB	192	146	0.02%	0.003%
59	9.243	2453	2458	2461	rBB	187	192	0.02%	0.003%
60	9.266	2462	2465	2469	rBB	160	164	0.02%	0.003%
61	9.337	2482	2487	2492	rBV	253	341	0.04%	0.006%
62	9.414	2497	2511	2532	rBV	331493	539994	68.54%	9.396%
63	9.562	2554	2557	2559	rBV2	274	214	0.03%	0.004%
64	9.668	2586	2590	2593	rBB	170	161	0.02%	0.003%
65	9.710	2599	2603	2607	rBB	160	152	0.02%	0.003%
66	9.771	2617	2622	2625	rBB	197	170	0.02%	0.003%
67	9.806	2629	2633	2638	rBB	192	202	0.03%	0.004%
68	9.873	2648	2654	2657	rBB	223	246	0.03%	0.004%
69	10.124	2729	2732	2735	rBV	172	159	0.02%	0.003%
70	10.153	2738	2741	2746	rVV	251	206	0.03%	0.004%
71	10.195	2749	2754	2758	rBB	248	207	0.03%	0.004%
72	10.433	2825	2828	2832	rBB	169	159	0.02%	0.003%
73	10.664	2896	2900	2904	rBB	276	247	0.03%	0.004%
74	10.684	2904	2906	2912	rBB	304	267	0.03%	0.005%
75	10.751	2915	2927	2945	rBV	258971	406508	51.60%	7.073%
76	10.883	2962	2968	2969	rBB	298	184	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
 Data File : VU052951.D
 Acq On : 03 Feb 2023 17:40
 Operator : JC/MD
 Sample : 01381-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.941	2983	2986	2991	rBB	220	238	0.03%	0.004%
78	10.970	2991	2995	2997	rBV2	274	244	0.03%	0.004%
79	11.015	3007	3009	3012	rBV	187	135	0.02%	0.002%
80	11.041	3013	3017	3018	rVV	256	132	0.02%	0.002%
81	11.237	3075	3078	3080	rVB	323	184	0.02%	0.003%
82	11.317	3098	3103	3105	rBV	243	251	0.03%	0.004%
83	11.394	3124	3127	3132	rBB	254	187	0.02%	0.003%
84	11.430	3133	3138	3140	rBV	198	225	0.03%	0.004%
85	11.500	3155	3160	3163	rBV	184	236	0.03%	0.004%
86	11.806	3243	3255	3269	rBV	331910	525110	66.65%	9.137%
87	11.951	3296	3300	3303	rVB2	481	364	0.05%	0.006%
88	11.973	3303	3307	3311	rBV	287	313	0.04%	0.005%
89	12.102	3344	3347	3349	rBV	211	165	0.02%	0.003%
90	12.111	3349	3350	3356	rVB	322	221	0.03%	0.004%
91	12.189	3361	3374	3398	rBV	366434	588386	74.68%	10.238%
92	13.369	3736	3741	3743	rBV	199	196	0.02%	0.003%
93	13.709	3844	3847	3851	rVB	345	216	0.03%	0.004%
94	13.848	3884	3890	3893	rBV2	717	704	0.09%	0.012%
95	14.150	3979	3984	3987	rBV2	424	518	0.07%	0.009%
96	14.217	4002	4005	4006	rBV	228	134	0.02%	0.002%
97	14.266	4017	4020	4025	rBV2	347	297	0.04%	0.005%
98	14.516	4095	4098	4099	rBV	258	146	0.02%	0.003%
99	14.568	4110	4114	4116	rBV2	410	287	0.04%	0.005%
100	14.893	4211	4215	4217	rBV2	428	372	0.05%	0.006%




Sum of corrected areas: 5747060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052951.D
Acq On : 03 Feb 2023 17:40
Operator : JC/MD
Sample : 01381-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

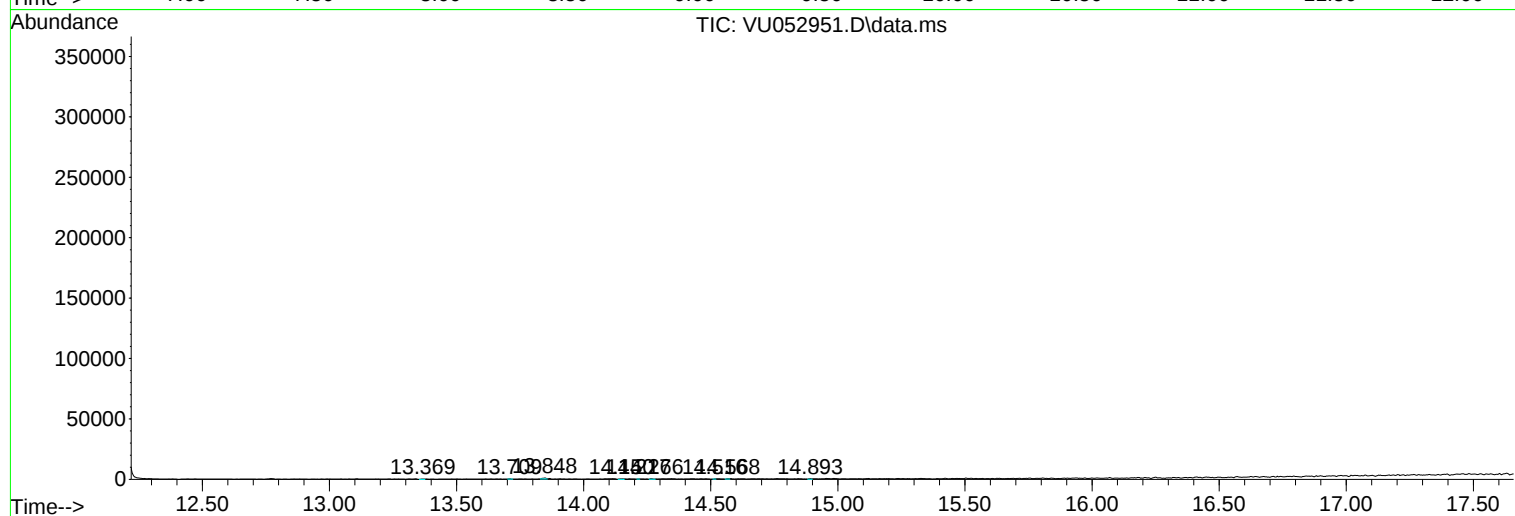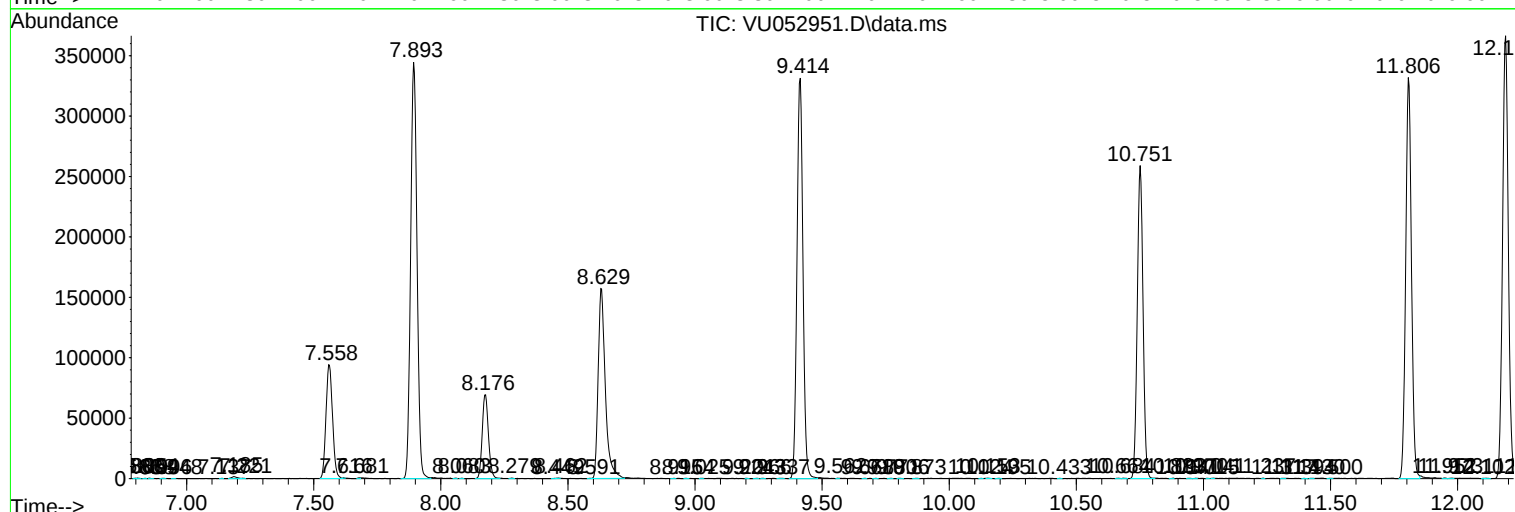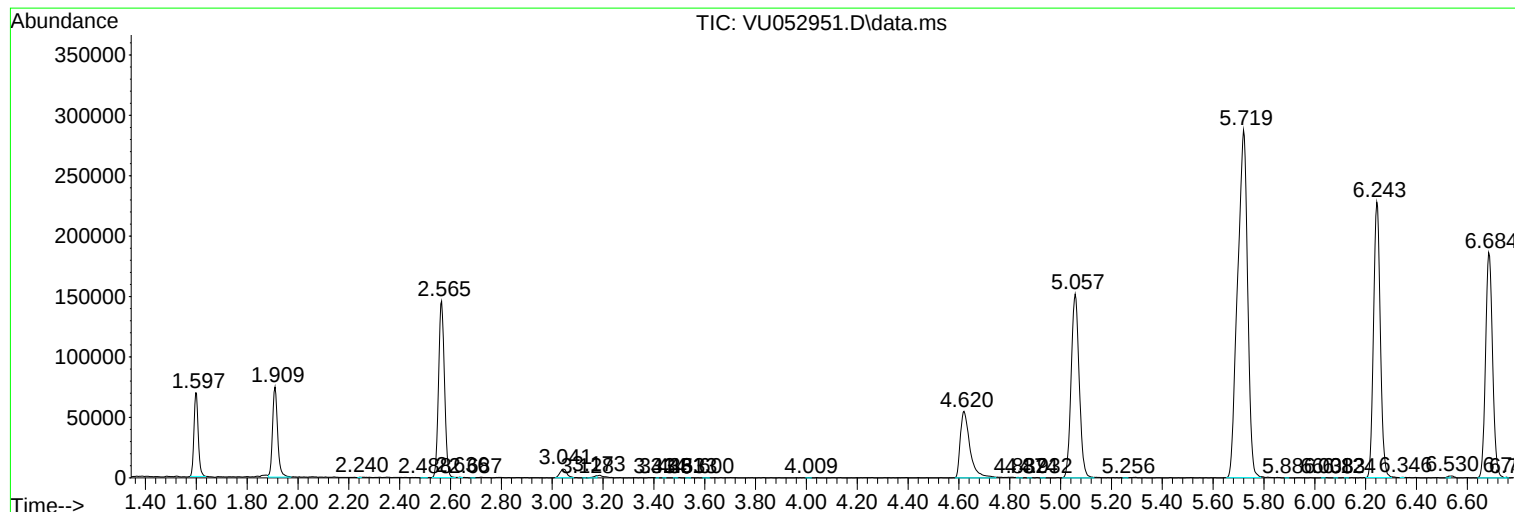

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052951.D
Acq On : 03 Feb 2023 17:40
Operator : JC/MD
Sample : 01381-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052951.D
Acq On : 03 Feb 2023 17:40
Operator : JC/MD
Sample : 01381-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------