
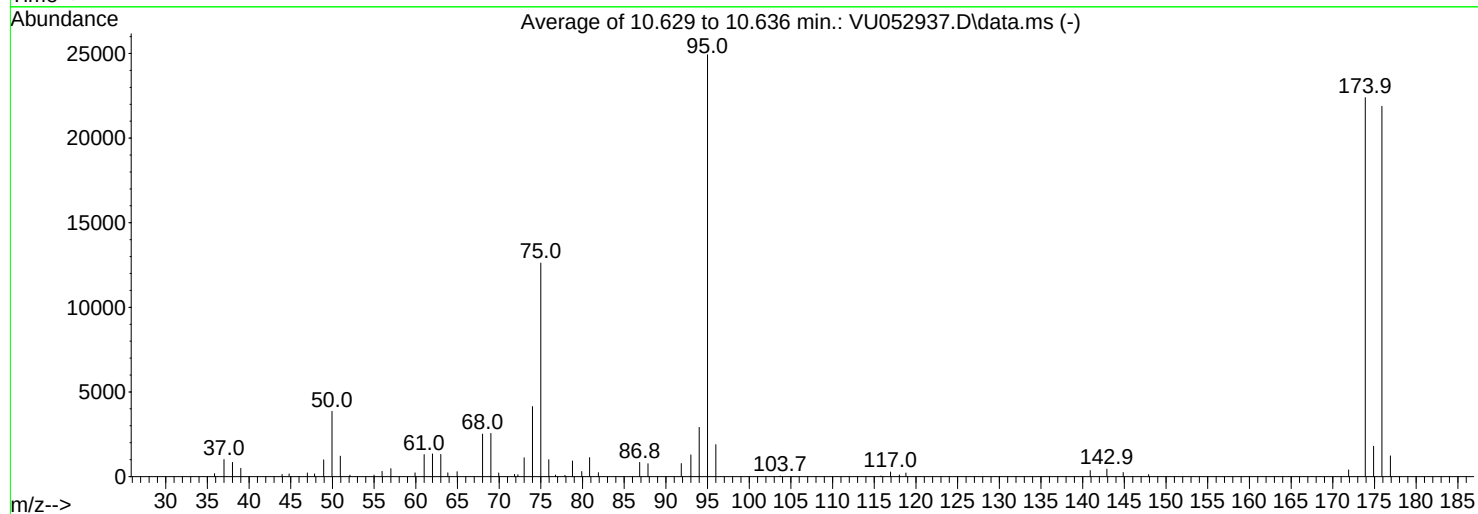


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020323\
Data File : VU052937.D
Acq On : 03 Feb 2023 11:27
Operator : JC/MD
Sample : BFB158
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB158

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Title : VOC Analysis
Last Update : Fri Feb 03 23:44:08 2023

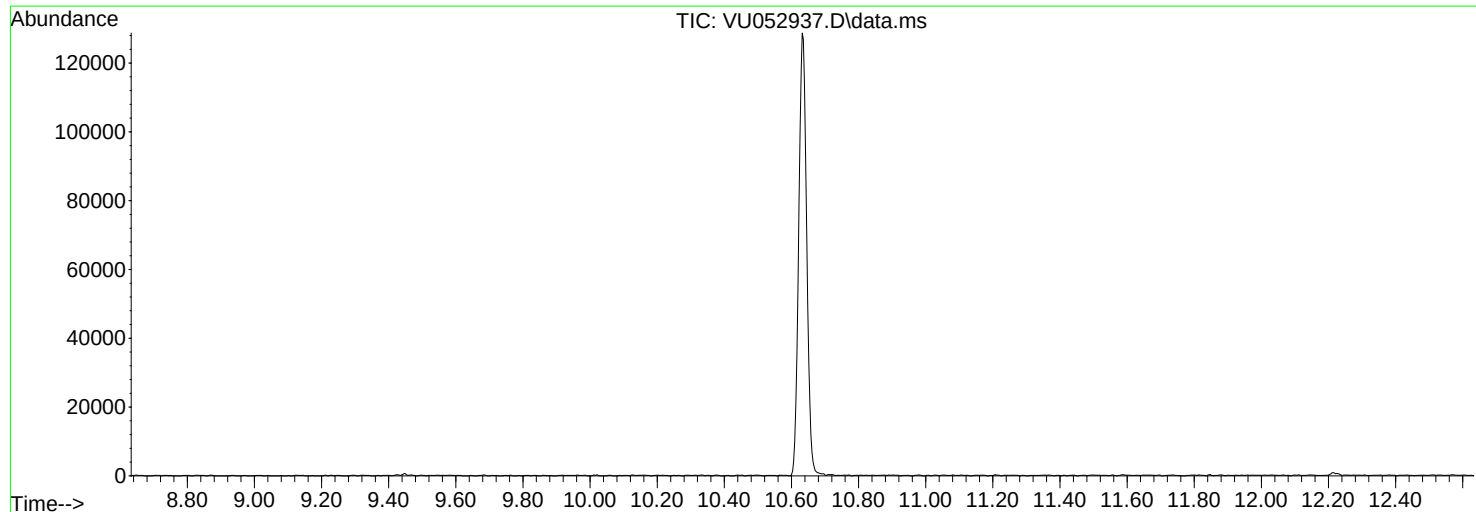

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.5	3851	PASS
75	95	30	80	50.6	12620	PASS
95	95	100	100	100.0	24925	PASS
96	95	5	9	7.6	1890	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.9	22397	PASS
175	174	5	9	8.0	1796	PASS
176	174	95	101	97.7	21888	PASS
177	176	5	9	5.6	1223	PASS

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB158

m/z	Abundance
35.80	161.0
37.00	932.0
38.00	795.0
39.00	400.0
43.90	133.0
44.80	173.0
47.00	239.0
47.80	163.0
48.90	875.0
50.00	3814.0
50.90	1219.0
52.10	104.0
55.90	243.0
57.00	542.0
59.90	253.0
61.00	1274.0
62.00	1413.0
63.00	1144.0
63.80	189.0
64.90	306.0
68.00	2456.0
69.00	2666.0
69.90	203.0
71.90	132.0
73.00	1017.0
74.00	3702.0
75.00	12403.0
75.90	1032.0
77.90	111.0
78.80	875.0
79.90	298.0
80.90	1012.0
81.90	232.0
86.90	878.0
87.80	706.0
91.90	706.0
93.00	1106.0
94.00	2613.0
95.00	23784.0
96.00	2037.0
103.70	111.0
115.80	103.0
116.90	220.0
118.80	205.0
140.90	392.0
142.90	415.0
144.80	238.0
147.90	108.0
171.90	301.0
173.90	20960.0
174.90	1727.0
175.90	20352.0
176.90	1268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB158

m/z	Abundance
35.90	167.0
37.00	1033.0
38.00	882.0
39.00	493.0
43.90	125.0
44.80	156.0
47.00	242.0
47.80	157.0
49.00	1045.0
50.00	3931.0
51.00	1221.0
52.10	123.0
55.00	137.0
56.00	321.0
57.00	450.0
59.90	222.0
61.00	1376.0
62.00	1398.0
63.00	1394.0
63.90	230.0
64.90	284.0
68.00	2640.0
69.00	2631.0
69.90	220.0
71.80	121.0
72.30	183.0
73.00	1138.0
74.00	4211.0
75.00	12980.0
76.00	1015.0
76.70	113.0
77.90	102.0
78.80	935.0
79.90	301.0
80.90	1150.0
81.90	231.0
86.90	837.0
87.90	803.0
91.90	782.0
93.00	1349.0
94.00	3059.0
95.00	25680.0
96.00	1942.0
117.00	274.0
118.00	134.0
118.80	226.0
140.90	377.0
142.90	428.0
144.90	230.0
147.90	122.0
171.90	431.0
173.90	23160.0
174.90	1841.0
175.90	22472.0
176.90	1241.0

Instrument :
MSVOA_U
ClientSampleId :
BFB158

m/z	Abundance
35.90	190.0
37.00	1051.0
38.00	844.0
39.00	568.0
44.00	132.0
44.80	128.0
47.00	167.0
47.90	136.0
49.00	1048.0
49.90	3809.0
51.00	1170.0
55.00	140.0
56.00	368.0
57.00	416.0
59.90	180.0
61.00	1265.0
62.00	1202.0
63.00	1393.0
63.90	241.0
65.00	278.0
68.00	2428.0
69.00	2343.0
70.00	224.0
71.80	118.0
72.20	133.0
73.00	1168.0
74.00	4509.0
75.00	12477.0
76.00	936.0
76.80	148.0
78.80	967.0
79.90	285.0
80.80	1198.0
81.90	220.0
86.80	806.0
87.80	770.0
91.80	816.0
93.00	1402.0
94.00	3042.0
95.00	25312.0
96.00	1690.0
117.00	306.0
118.00	161.0
118.80	206.0
140.90	304.0
142.90	466.0
144.90	248.0
147.90	119.0
171.90	455.0
173.90	23072.0
174.90	1819.0
175.90	22840.0
176.90	1159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB158