
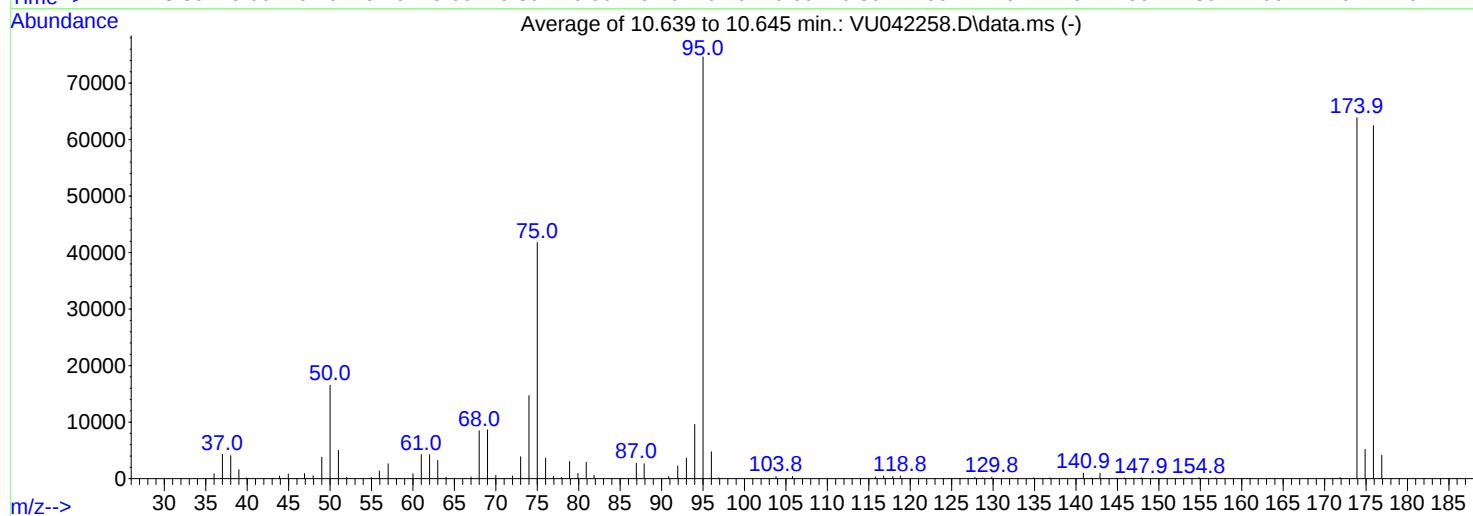


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020421\
 Data File : VU042258.D
 Acq On : 04 Feb 2021 09:16
 Operator : SY/MD
 Sample : BFB43
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB43

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR012021WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Feb 05 02:23:43 2021

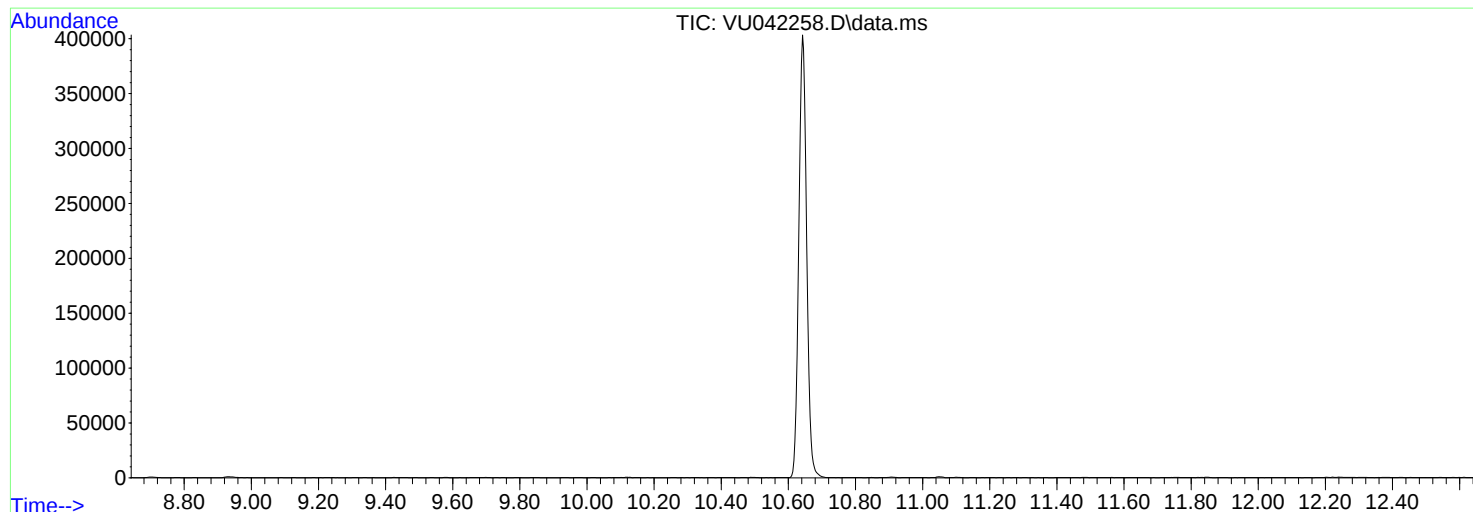

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	16536	PASS
75	95	30	80	56.0	41787	PASS
95	95	100	100	100.0	74637	PASS
96	95	5	9	6.4	4756	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.6	63883	PASS
175	174	5	9	8.1	5195	PASS
176	174	95	101	97.8	62461	PASS
177	176	5	9	6.6	4131	PASS

m/z	Abundance
36.00	798.0
37.00	4315.0
38.00	4048.0
39.00	1584.0
39.90	142.0
43.00	105.0
44.00	736.0
44.90	869.0
46.90	843.0
47.90	520.0
49.00	3753.0
50.00	16512.0
51.00	4948.0
52.00	251.0
54.90	275.0
55.90	1467.0
57.00	2639.0
57.90	109.0
60.00	861.0
61.00	4184.0
62.00	4086.0
63.00	3205.0
64.00	262.0
67.00	316.0
68.00	8040.0
69.00	8215.0
70.00	561.0
72.00	516.0
73.00	3750.0
74.00	14377.0
75.00	40928.0
76.00	3553.0
77.00	431.0
77.90	228.0
78.90	2971.0
79.90	866.0
80.90	2858.0
81.90	604.0
87.00	2631.0
87.90	2543.0
90.80	363.0
91.90	2241.0
93.00	3466.0
94.00	9316.0
95.00	72768.0
96.00	4801.0
96.90	167.0
103.80	367.0
105.80	368.0
115.80	303.0
116.80	437.0
117.90	365.0
118.80	447.0
127.80	258.0
128.70	165.0
129.90	252.0
134.90	165.0
136.90	136.0
140.90	887.0
141.80	107.0
142.90	923.0
144.80	115.0
145.90	144.0
147.70	179.0
154.80	208.0
156.80	105.0
158.90	112.0
171.80	159.0
173.90	60176.0
174.90	5008.0
175.90	58888.0
176.90	3945.0
178.00	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	875.0
37.00	4426.0
38.00	4236.0
39.00	1691.0
39.90	151.0
43.00	108.0
43.90	730.0
44.90	870.0
46.90	975.0
48.00	519.0
49.00	3922.0
50.00	17056.0
51.00	5201.0
52.00	256.0
54.90	244.0
55.90	1402.0
57.00	2733.0
60.00	935.0
61.00	4399.0
62.00	4366.0
63.00	3344.0
64.00	287.0
67.00	314.0
68.00	8740.0
69.00	8998.0
70.00	610.0
72.00	491.0
73.00	4036.0
74.00	15192.0
75.00	43104.0
76.00	3786.0
76.90	423.0
77.90	232.0
78.90	3151.0
79.90	996.0
80.90	2981.0
81.90	620.0
87.00	2835.0
87.90	2761.0
90.80	386.0
91.90	2304.0
93.00	3748.0
94.00	9907.0
95.00	77128.0
96.00	4850.0
96.90	155.0
103.80	427.0
105.80	392.0
115.80	324.0
116.80	481.0
117.90	392.0
118.80	511.0
127.80	278.0
128.70	165.0
129.80	285.0
134.90	201.0
136.80	142.0
140.90	1008.0
141.80	124.0
142.90	1014.0
144.90	108.0
145.90	141.0
147.90	201.0
154.90	214.0
156.90	120.0
160.70	104.0
171.90	206.0
173.90	65936.0
174.90	5375.0
175.90	64464.0
176.90	4251.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	863.0
37.00	4158.0
38.00	3965.0
39.00	1500.0
39.90	129.0
43.90	698.0
45.00	775.0
46.90	951.0
48.00	485.0
49.00	3719.0
50.00	16040.0
51.00	4914.0
52.00	232.0
55.00	206.0
56.00	1241.0
57.00	2518.0
60.00	875.0
61.00	4226.0
62.00	4255.0
63.00	3120.0
64.00	279.0
67.00	271.0
68.00	8619.0
69.00	8688.0
70.00	659.0
72.00	433.0
73.00	3869.0
74.00	14547.0
75.00	41328.0
76.00	3503.0
76.90	431.0
77.90	255.0
78.90	2942.0
79.90	980.0
80.90	2863.0
81.80	599.0
86.90	2718.0
87.90	2649.0
90.90	361.0
92.00	2204.0
93.00	3700.0
94.00	9589.0
95.00	74016.0
96.00	4617.0
96.90	121.0
103.80	422.0
105.80	393.0
115.80	298.0
116.80	494.0
117.90	351.0
118.80	510.0
127.80	260.0
128.80	138.0
129.80	277.0
134.90	175.0
136.80	142.0
140.90	1037.0
141.90	140.0
142.90	957.0
145.80	117.0
147.90	256.0
154.90	210.0
156.80	118.0
160.70	110.0
171.90	254.0
173.90	65536.0
174.90	5201.0
175.90	64032.0
176.90	4198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
43.90	267.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43