

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020519\
 Data File : VU029345.D
 Acq On : 05 Feb 2019 13:31
 Operator : JC/SP
 Sample : I.BLK
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK49

Quant Time: Feb 08 10:43:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U020519DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Feb 08 10:20:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.74	96	52421	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	20399	1.00	ug/l	0.00
Spiked Amount 1.000			Recovery	=	100.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	20865	0.99	ug/l	0.00
Spiked Amount 1.000			Recovery	=	99.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020519\
Data File : VU029345.D
Acq On : 05 Feb 2019 13:31
Operator : JC/SP
Sample : I.BLK
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK49

Quant Time: Feb 08 10:43:20 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U020519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Feb 08 10:20:02 2019
Response via : Initial Calibration




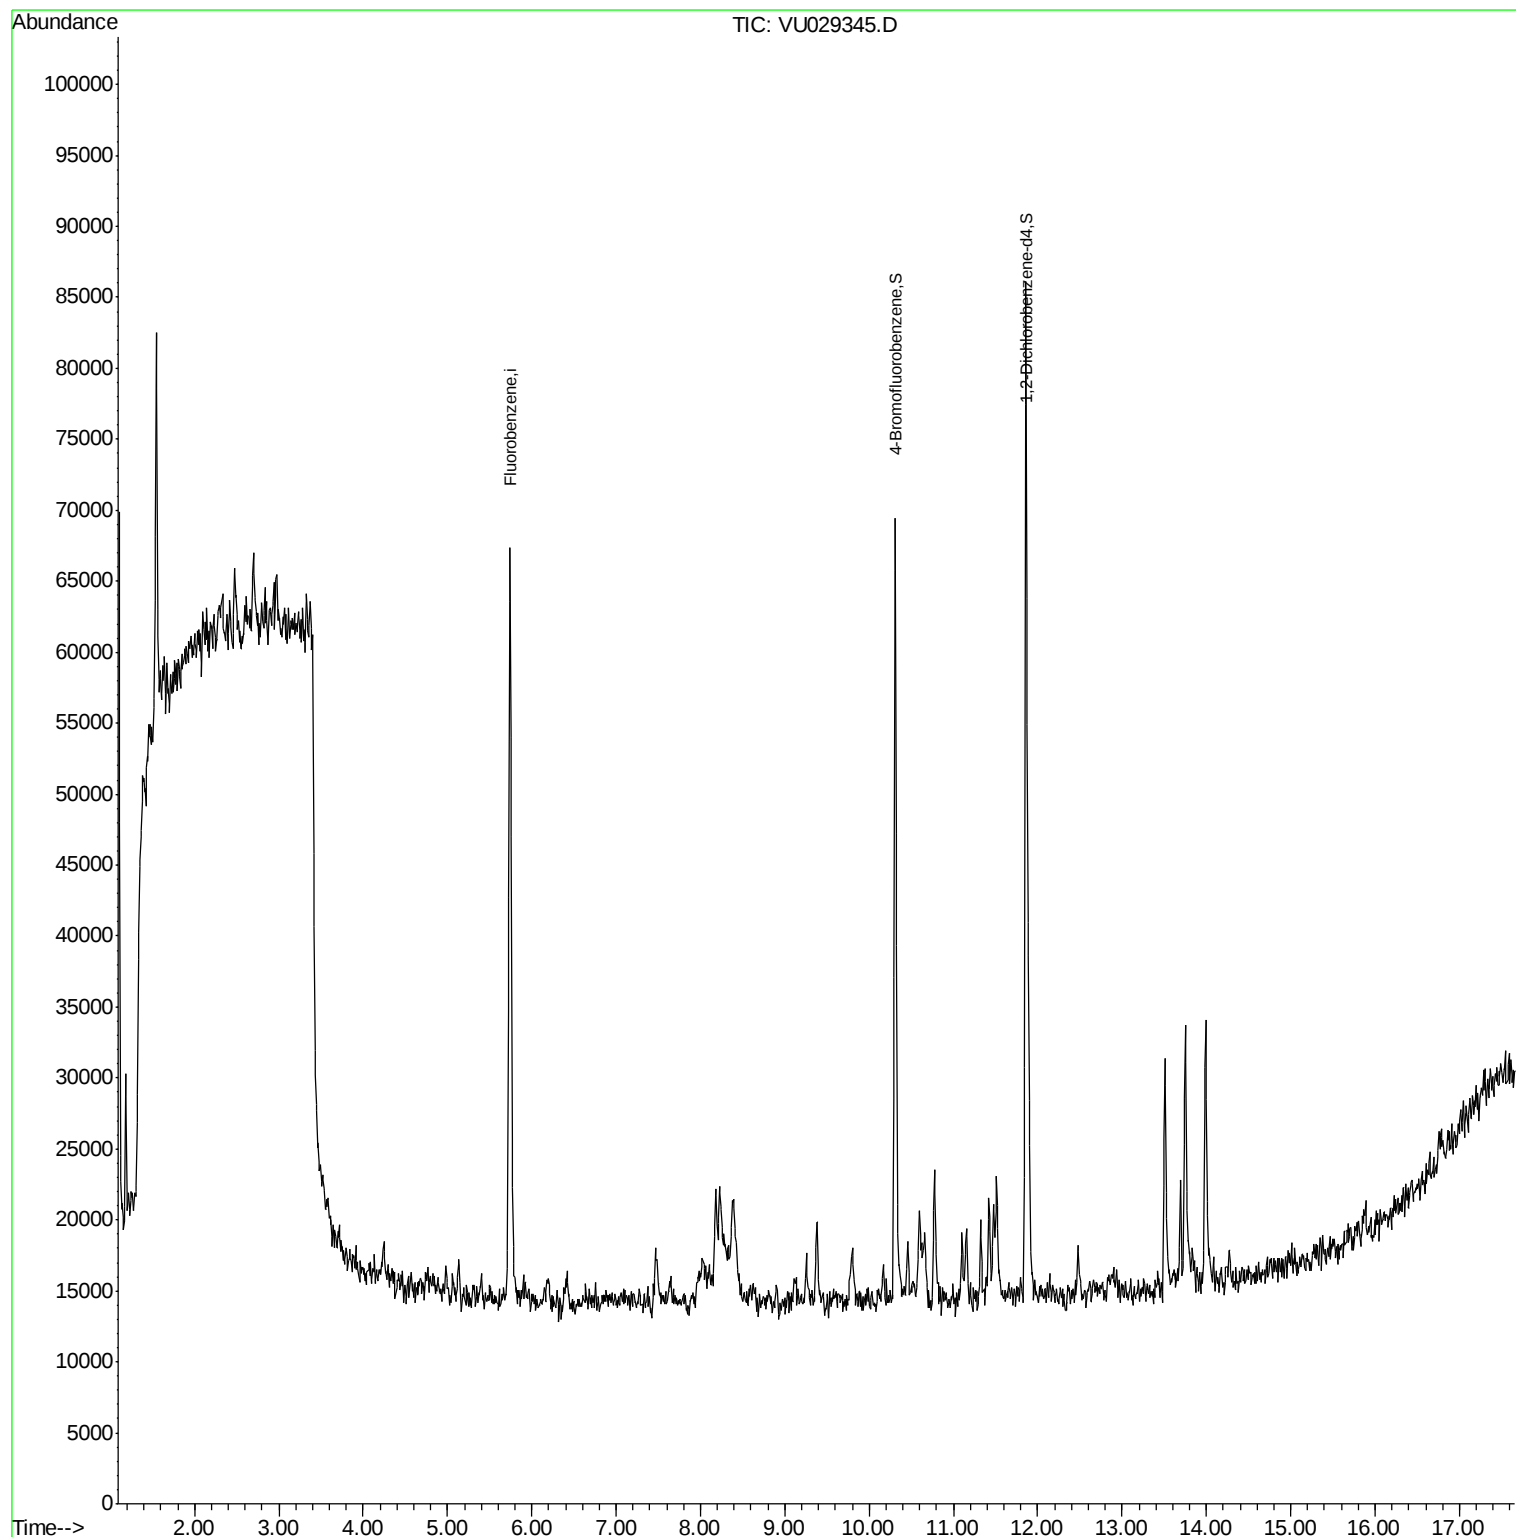


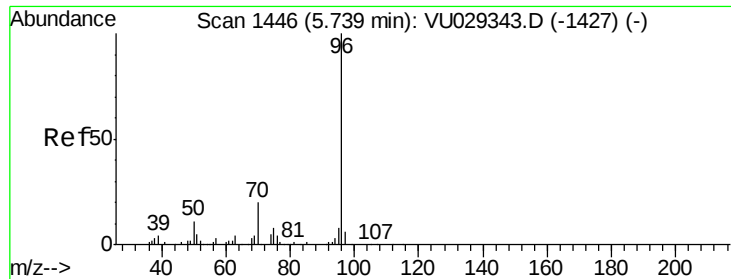

#1
 Fluorobenzene
 Concen: 1.000 ug/l
 RT: 5.74 min Scan# 1447
 Delta R.T. 0.00 min
 Lab File: VU029345.D
 Acq: 05 Feb 2019 13:31




Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK49


Tot Ion:	96	Resp:	52421
Ion	Ratio	Lower	Upper
96	100		
70	21.1	16.2	24.2
95	8.9	7.4	11.2
97	6.2	0.0	0.0#

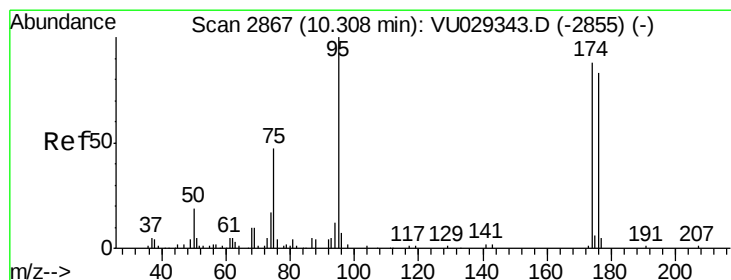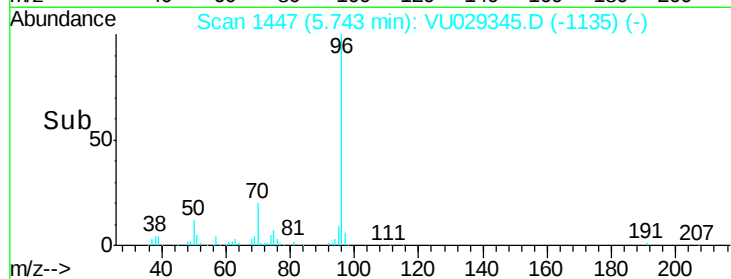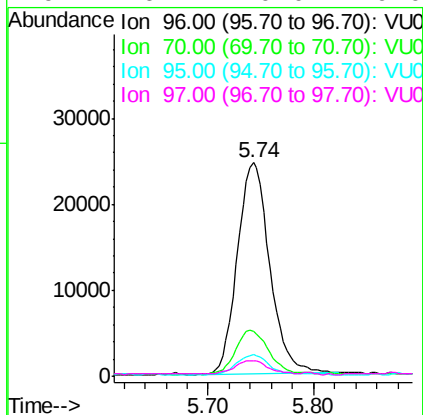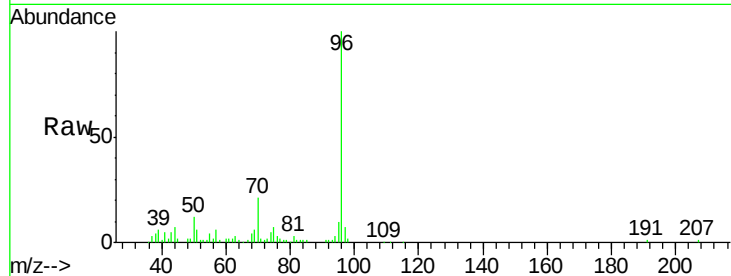

#57
 4-Bromofluorobenzene
 Concen: Below ug/l
 RT: 10.31 min Scan# 2867
 Delta R.T. 0.00 min
 Lab File: VU029345.D
 Acq: 05 Feb 2019 13:31

Tgt Ion:	95	Resp:	20399
Ion	Ratio	Lower	Upper
95	100		
174	84.1	64.2	96.2
176	82.1	62.3	93.5

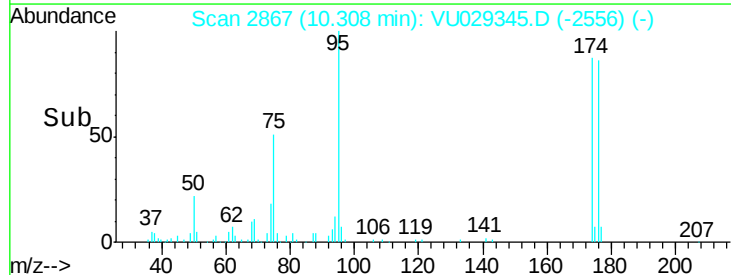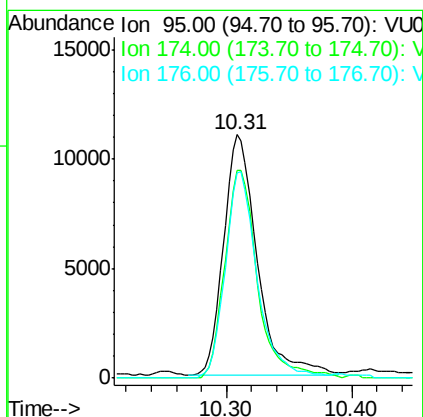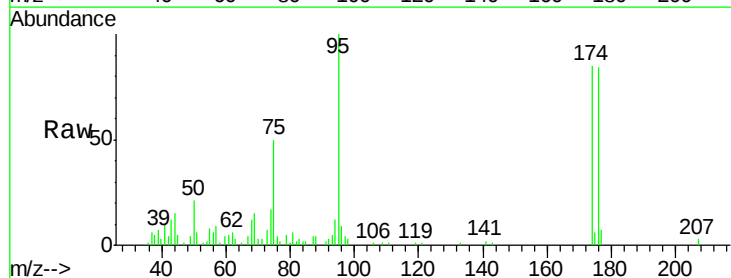

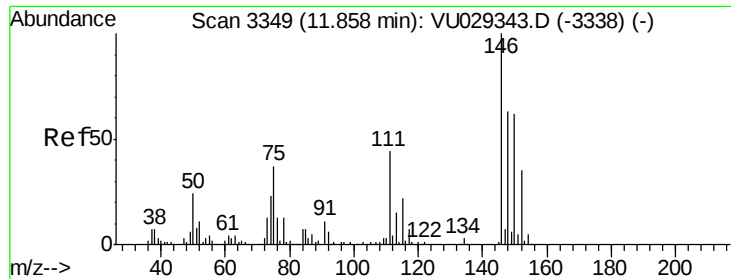

#68
 1,2-Dichlorobenzene-d4
 Concen: Below ug/l
 RT: 11.86 min Scan# 3350
 Delta R.T. 0.00 min
 Lab File: VU029345.D
 Acq: 05 Feb 2019 13:31

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK49

Tot Ion	Ratio	Lower	Upper
152	100		
115	61.3	0.0	133.4
150	152.9	0.0	670.8

