

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020519\
Data File : VU029348.D
Acq On : 05 Feb 2019 15:25
Operator : JC/SP
Sample : VU0205WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK50

Quant Time: Feb 08 11:18:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U020519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Feb 08 10:52:46 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.74	96	52121	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.31	95	19510	0.96	ug/l	0.00
Spiked Amount	1.000		Recovery	=	96.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	19686	0.94	ug/l	0.00
Spiked Amount	1.000		Recovery	=	94.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020519\
Data File : VU029348.D
Acq On : 05 Feb 2019 15:25
Operator : JC/SP
Sample : VU0205WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK50

Quant Time: Feb 08 11:18:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U020519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Feb 08 10:52:46 2019
Response via : Initial Calibration

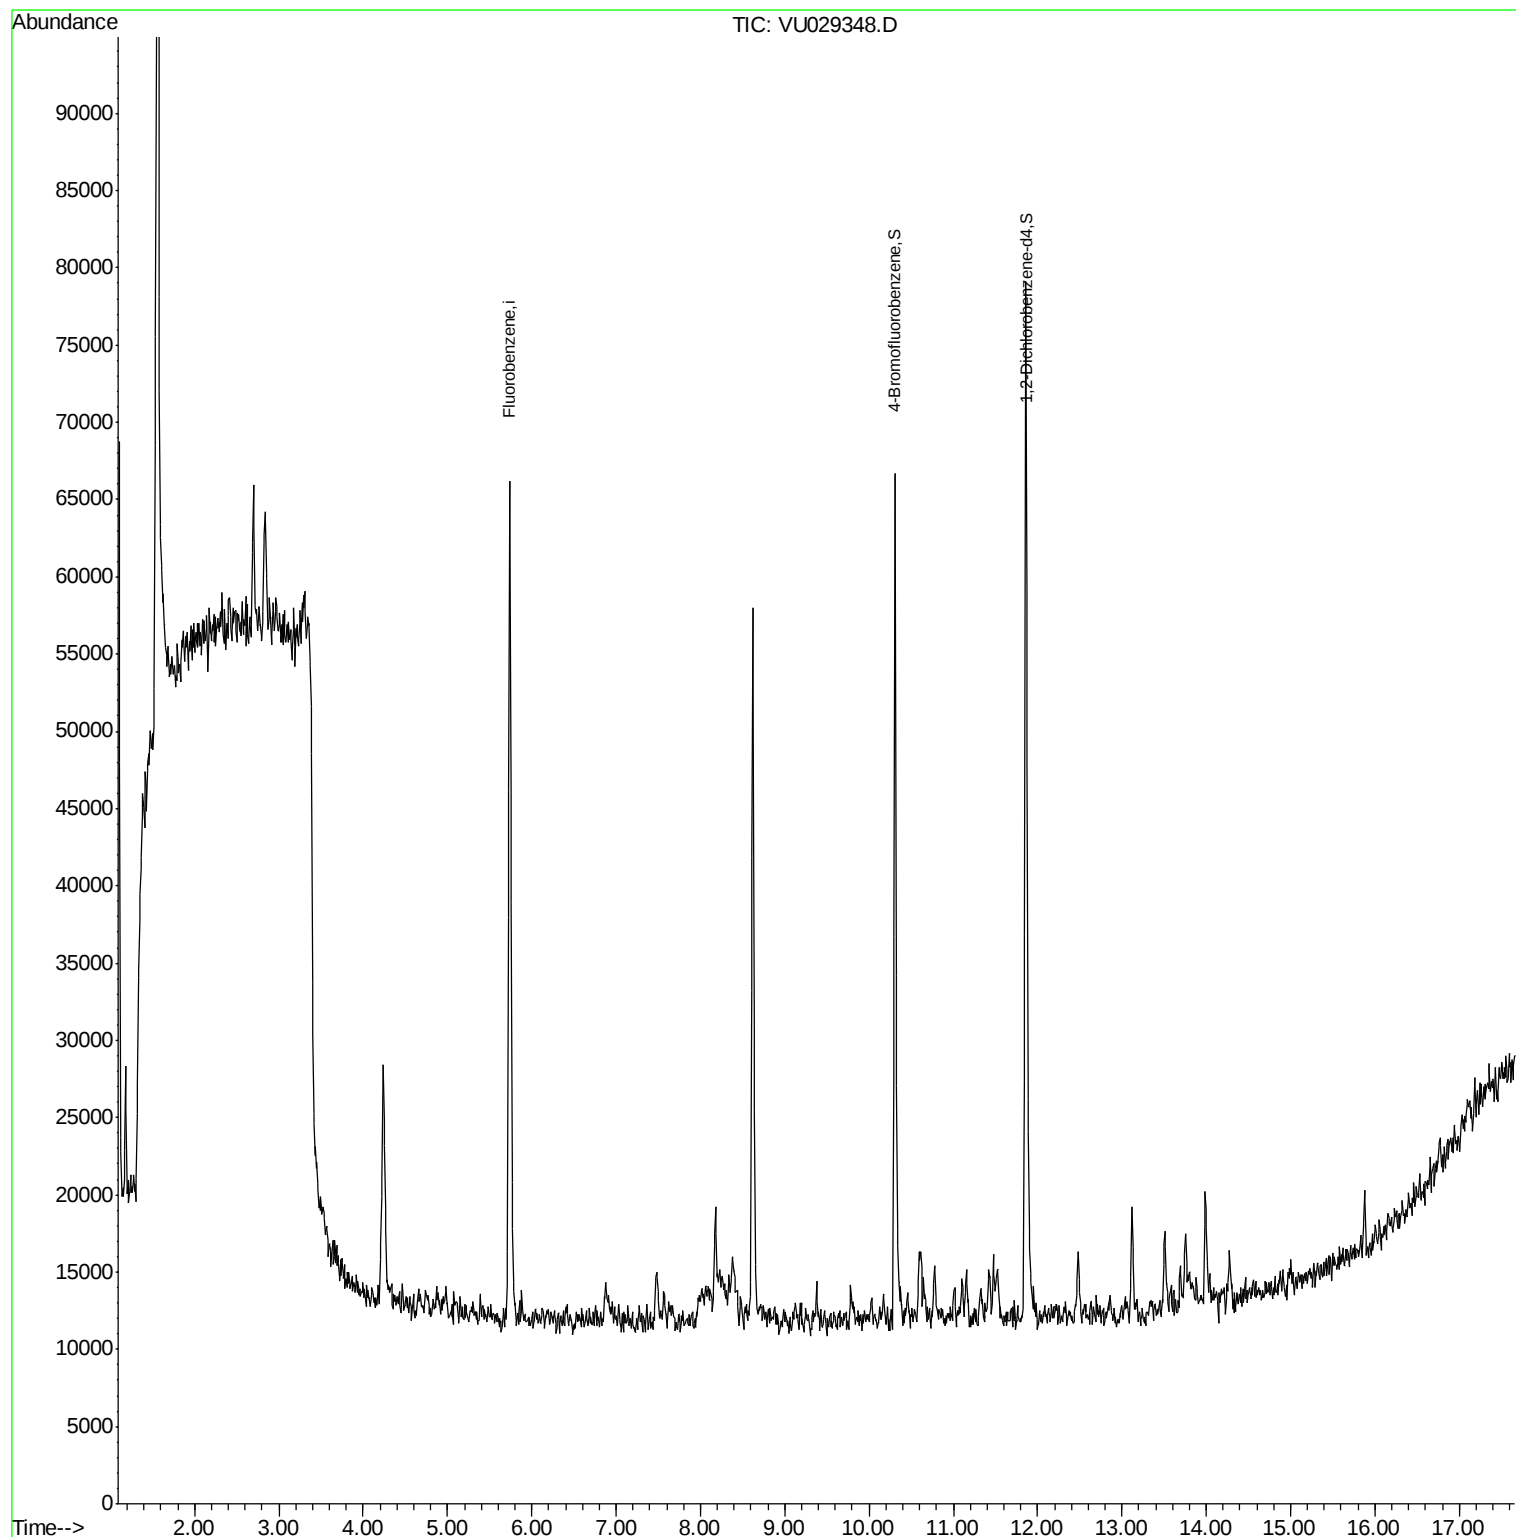

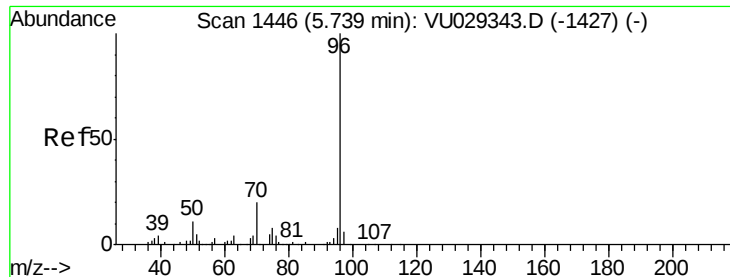

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.74 min Scan# 1446

Delta R.T. 0.00 min

Lab File: VU029348.D

Acq: 05 Feb 2019 15:25

Instrument :

MSVOA_U

ClientSampleId :

VBLK50

Tot Ion: 96 Resp: 52121


Ion Ratio Lower Upper

96 100

70 19.9 16.2 24.2

95 10.0 7.4 11.2

97 5.8 0.0 0.0#



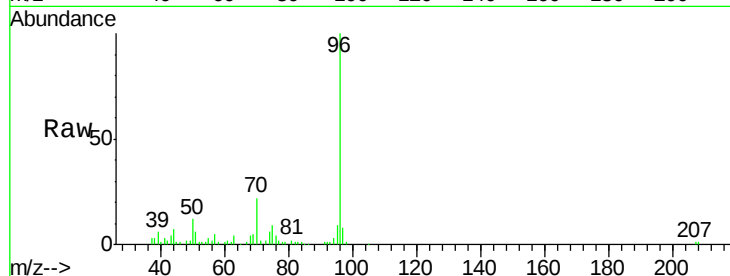


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

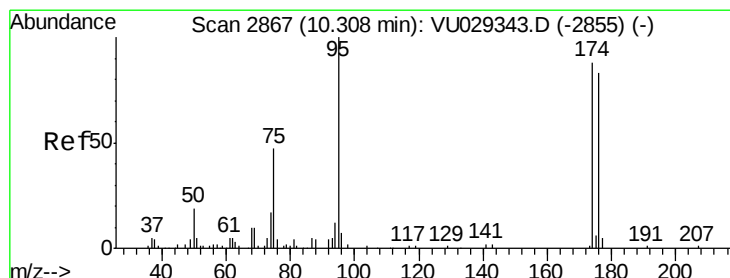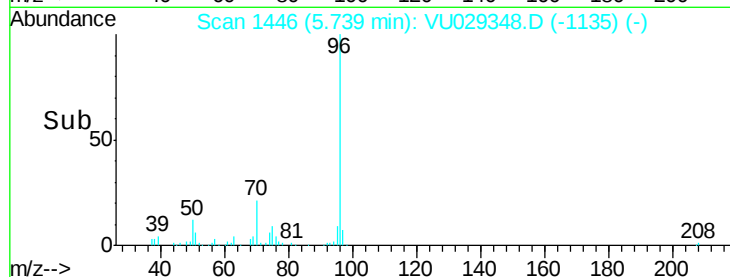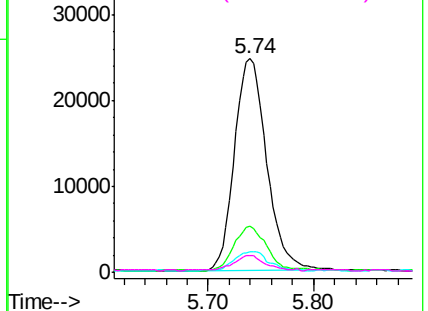

#57

4-Bromofluorobenzene

Concen: Below ug/l

RT: 10.31 min Scan# 2867

Delta R.T. 0.00 min

Lab File: VU029348.D

Acq: 05 Feb 2019 15:25


Tgt Ion: 95 Resp: 19510

Ion Ratio Lower Upper

95 100

174 86.0 64.2 96.2



176 83.6 62.3 93.5

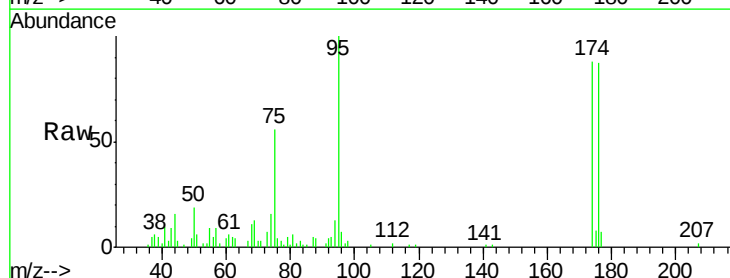


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

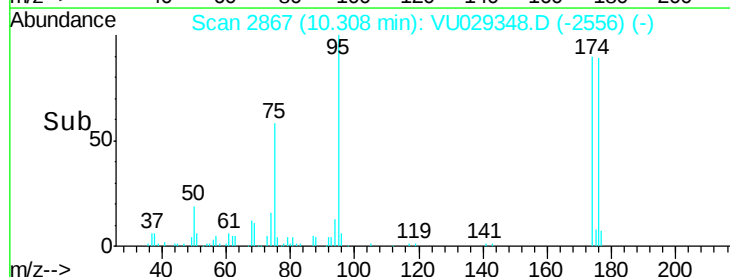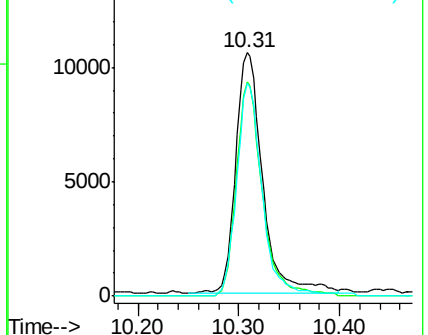


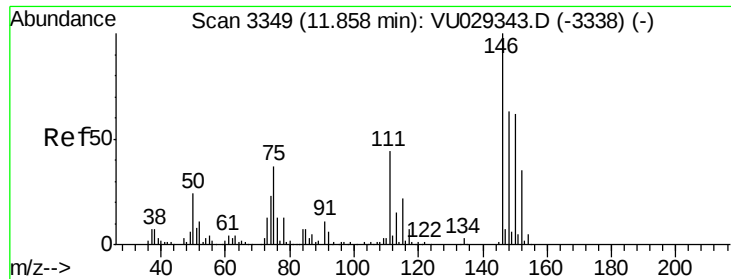

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.86 min Scan# 3350
 Delta R.T. 0.00 min
 Lab File: VU029348.D
 Acq: 05 Feb 2019 15:25

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK50

Tot Ion	Ratio	Lower	Upper
152	100		
115	61.0	0.0	133.4
150	153.9	0.0	670.8

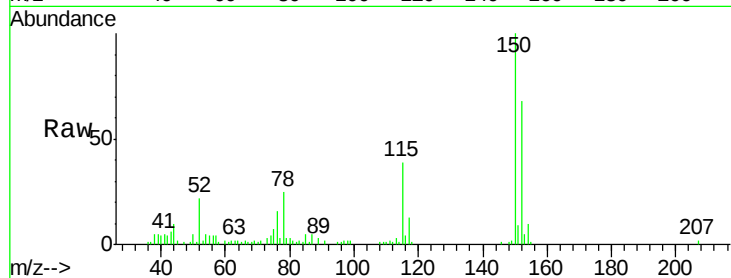

Abundance Ion 152.00 (151.70 to 152.70): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 150.00 (149.70 to 150.70): V

