


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU020519\
 Data File : VU029338.D
 Acq On : 05 Feb 2019 09:53
 Operator : JC/SP
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U020519DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Feb 08 10:52:46 2019

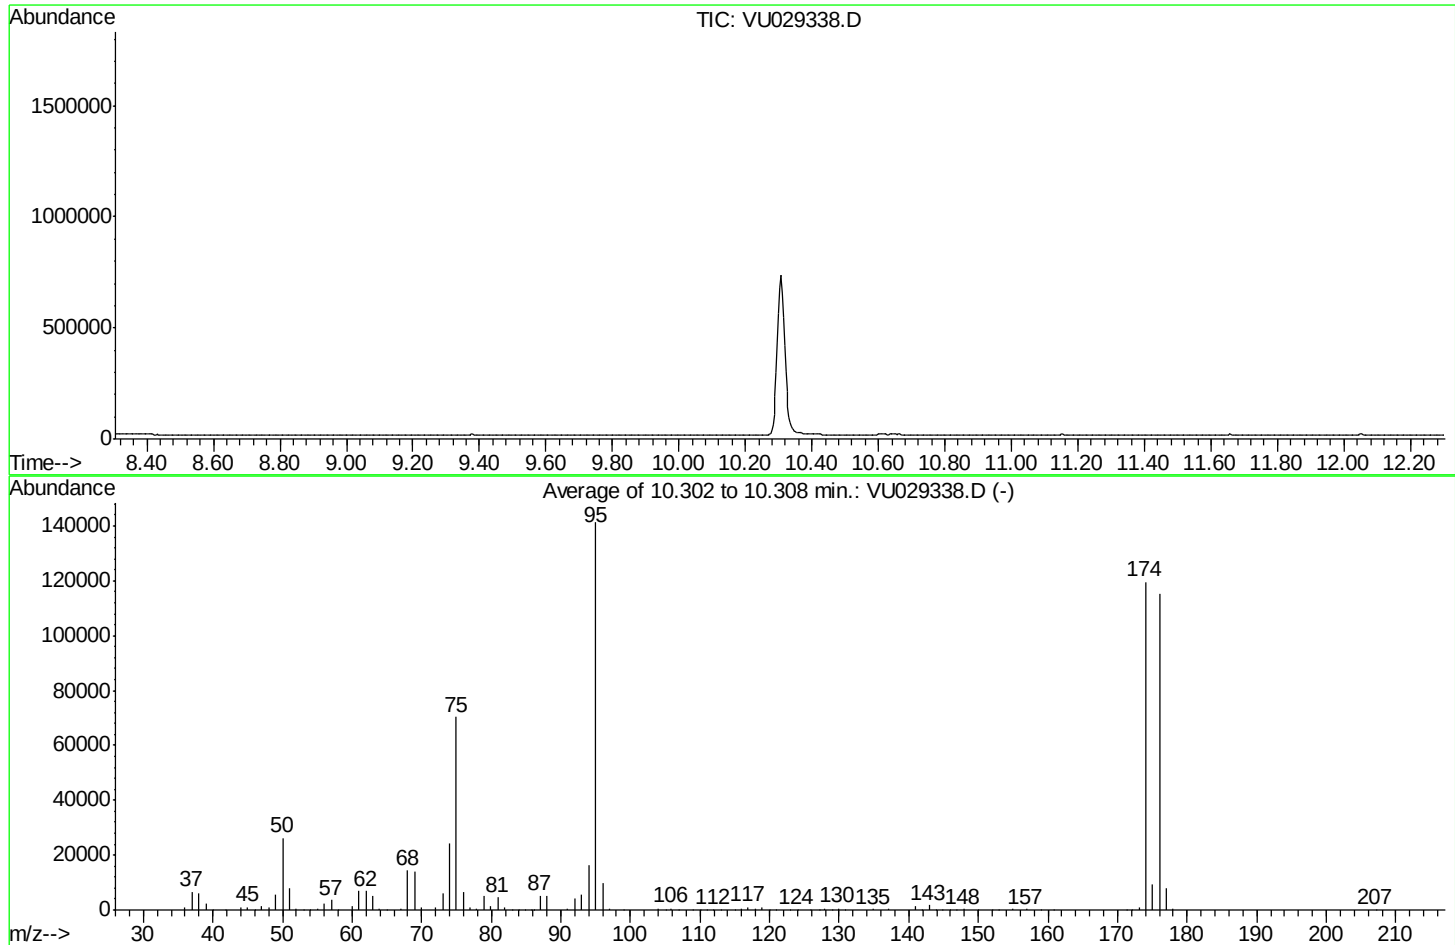

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	26241	PASS
75	95	30	60	49.8	70389	PASS
95	95	100	100	100.0	141312	PASS
96	95	5	9	6.9	9690	PASS
173	174	0.00	2	0.9	1135	PASS
174	95	50	100	84.6	119570	PASS
175	174	5	9	7.6	9139	PASS
176	174	95	101	96.6	115480	PASS
177	176	5	9	6.8	7842	PASS