

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020521\
 Data File : VU042281.D
 Acq On : 05 Feb 2021 16:22
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M

Title : VOC Analysis

Signal : TIC: VU042281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	103	rVB	104210	120598	13.69%	1.761%
2	1.919	171	180	196	rVB	80570	104966	11.91%	1.533%
3	2.501	359	361	364	rVB	226	124	0.01%	0.002%
4	2.575	371	384	413	rBV	196114	337440	38.30%	4.927%
5	2.806	449	456	464	rBV2	322	572	0.06%	0.008%
6	2.841	464	467	472	rVB2	190	159	0.02%	0.002%
7	2.999	511	516	520	rBV2	212	219	0.02%	0.003%
8	3.060	527	535	544	rVV3	772	1147	0.13%	0.017%
9	3.112	548	551	555	rVB2	212	141	0.02%	0.002%
10	3.935	803	807	816	rBV	100	159	0.02%	0.002%
11	4.401	950	952	956	rVB	203	137	0.02%	0.002%
12	4.446	963	966	970	rVB2	211	177	0.02%	0.003%
13	4.642	1010	1027	1066	rBV	85478	253630	28.79%	3.703%
14	4.883	1098	1102	1104	rBV	151	142	0.02%	0.002%
15	4.909	1105	1110	1115	rVV2	241	305	0.03%	0.004%
16	5.073	1143	1161	1180	rVV	160166	351215	39.86%	5.128%
17	5.195	1196	1199	1204	rBV3	223	168	0.02%	0.002%
18	5.735	1345	1367	1395	rBV2	322946	881113	100.00%	12.864%
19	5.999	1447	1449	1453	rVB	308	180	0.02%	0.003%
20	6.050	1462	1465	1468	rVB2	254	213	0.02%	0.003%
21	6.176	1501	1504	1507	rVB2	325	201	0.02%	0.003%
22	6.195	1507	1510	1513	rBV	389	327	0.04%	0.005%
23	6.259	1516	1530	1550	rBV	260475	492156	55.86%	7.186%
24	6.459	1590	1592	1595	rBV2	201	128	0.01%	0.002%
25	6.542	1610	1618	1627	rVB8	1824	3185	0.36%	0.047%
26	6.584	1627	1631	1634	rVB3	232	172	0.02%	0.003%
27	6.700	1653	1667	1695	rBV2	205699	399302	45.32%	5.830%
28	6.806	1695	1700	1701	rBV3	598	418	0.05%	0.006%
29	7.041	1769	1773	1774	rBV	215	175	0.02%	0.003%
30	7.182	1815	1817	1818	rVV	244	103	0.01%	0.002%
31	7.192	1818	1820	1823	rVB2	288	162	0.02%	0.002%
32	7.574	1926	1939	1961	rBV	125175	218881	24.84%	3.196%
33	7.767	1994	1999	2000	rBV	167	138	0.02%	0.002%
34	7.806	2003	2011	2025	rVB5	1166	2129	0.24%	0.031%
35	7.906	2029	2042	2060	rBV	397576	688432	78.13%	10.051%
36	8.089	2096	2099	2106	rVB2	385	433	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020521\
 Data File : VU042281.D
 Acq On : 05 Feb 2021 16:22
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis

37	8.189	2118	2130	2150	rBV	86341	150084	17.03%	2.191%
38	8.317	2166	2170	2173	rVB	169	174	0.02%	0.003%
39	8.343	2175	2178	2182	rVV2	174	158	0.02%	0.002%
40	8.410	2195	2199	2205	rBV3	337	399	0.05%	0.006%
41	8.449	2209	2211	2214	rVB2	181	107	0.01%	0.002%
42	8.475	2214	2219	2220	rBV	162	157	0.02%	0.002%
43	8.562	2242	2246	2250	rVB2	603	423	0.05%	0.006%
44	8.645	2256	2272	2305	rBV	295179	557626	63.29%	8.141%
45	8.819	2323	2326	2330	rVB2	160	105	0.01%	0.002%
46	8.870	2339	2342	2343	rBV2	220	115	0.01%	0.002%
47	8.960	2365	2370	2372	rBV	135	131	0.01%	0.002%
48	9.426	2502	2515	2546	rVV	356092	588268	66.76%	8.589%
49	9.703	2593	2601	2609	rVB4	1904	2539	0.29%	0.037%
50	9.902	2660	2663	2667	rBV	178	118	0.01%	0.002%
51	9.928	2669	2671	2678	rVB	261	163	0.02%	0.002%
52	10.041	2704	2706	2710	rVB2	228	150	0.02%	0.002%
53	10.066	2710	2714	2717	rBV	246	191	0.02%	0.003%
54	10.124	2723	2732	2743	rVB4	2692	4013	0.46%	0.059%
55	10.208	2755	2758	2763	rBV2	184	139	0.02%	0.002%
56	10.317	2789	2792	2798	rVB2	179	167	0.02%	0.002%
57	10.381	2808	2812	2814	rBV2	181	140	0.02%	0.002%
58	10.452	2832	2834	2837	rBV	134	103	0.01%	0.002%
59	10.610	2879	2883	2889	rBV2	253	242	0.03%	0.004%
60	10.690	2906	2908	2912	rVB	217	121	0.01%	0.002%
61	10.767	2918	2932	2951	rVB	270386	440987	50.05%	6.438%
62	10.838	2951	2954	2958	rBV	140	142	0.02%	0.002%
63	10.896	2970	2972	2977	rVB3	246	188	0.02%	0.003%
64	11.102	3027	3036	3045	rVV4	2111	3296	0.37%	0.048%
65	11.195	3063	3065	3068	rVB2	200	110	0.01%	0.002%
66	11.500	3157	3160	3162	rBV2	204	116	0.01%	0.002%
67	11.603	3187	3192	3193	rBV	212	127	0.01%	0.002%
68	11.754	3232	3239	3247	rBV3	1968	2947	0.33%	0.043%
69	11.822	3247	3260	3278	rBV	360002	573198	65.05%	8.369%
70	11.957	3300	3302	3307	rVB	202	190	0.02%	0.003%
71	12.066	3333	3336	3339	rBV2	172	117	0.01%	0.002%
72	12.201	3365	3378	3395	rBV	381688	629144	71.40%	9.186%
73	12.423	3443	3447	3451	rBV2	292	254	0.03%	0.004%
74	12.455	3454	3457	3462	rVB	238	178	0.02%	0.003%
75	12.520	3475	3477	3482	rVB2	190	122	0.01%	0.002%
76	12.626	3507	3510	3514	rBV	206	139	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020521\
 Data File : VU042281.D
 Acq On : 05 Feb 2021 16:22
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis

77	12.667	3521	3523	3529	rVB	253	179	0.02%	0.003%
78	12.786	3556	3560	3564	rBV2	277	230	0.03%	0.003%
79	12.957	3610	3613	3617	rBV	171	131	0.01%	0.002%
80	13.095	3652	3656	3657	rBV	164	123	0.01%	0.002%
81	13.147	3669	3672	3674	rBV	163	116	0.01%	0.002%
82	13.230	3692	3698	3699	rBV2	542	505	0.06%	0.007%
83	13.269	3702	3710	3712	rBV2	236	264	0.03%	0.004%
84	13.314	3721	3724	3727	rBB2	171	114	0.01%	0.002%
85	13.362	3737	3739	3742	rVB	230	117	0.01%	0.002%
86	13.674	3833	3836	3837	rBV2	236	160	0.02%	0.002%
87	13.764	3862	3864	3866	rBV	196	124	0.01%	0.002%
88	13.851	3881	3891	3904	rVB2	13767	21150	2.40%	0.309%
89	13.902	3904	3907	3910	rBV2	268	218	0.02%	0.003%
90	14.031	3940	3947	3954	rVB4	6267	7723	0.88%	0.113%
91	14.204	3999	4001	4005	rVB	245	153	0.02%	0.002%
92	14.246	4011	4014	4021	rVB	201	145	0.02%	0.002%
93	14.323	4036	4038	4039	rBV	262	103	0.01%	0.002%
94	14.368	4049	4052	4055	rBV	230	103	0.01%	0.002%
95	14.413	4063	4066	4068	rBV3	255	222	0.03%	0.003%
96	14.603	4123	4125	4130	rVB2	319	194	0.02%	0.003%
97	14.638	4134	4136	4139	rBV2	294	208	0.02%	0.003%
98	14.661	4139	4143	4146	rBV2	337	263	0.03%	0.004%
99	15.015	4250	4253	4256	rBV2	257	187	0.02%	0.003%
100	16.690	4772	4774	4775	rBV	700	324	0.04%	0.005%




Sum of corrected areas: 6849291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020521\
Data File : VU042281.D
Acq On : 05 Feb 2021 16:22
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

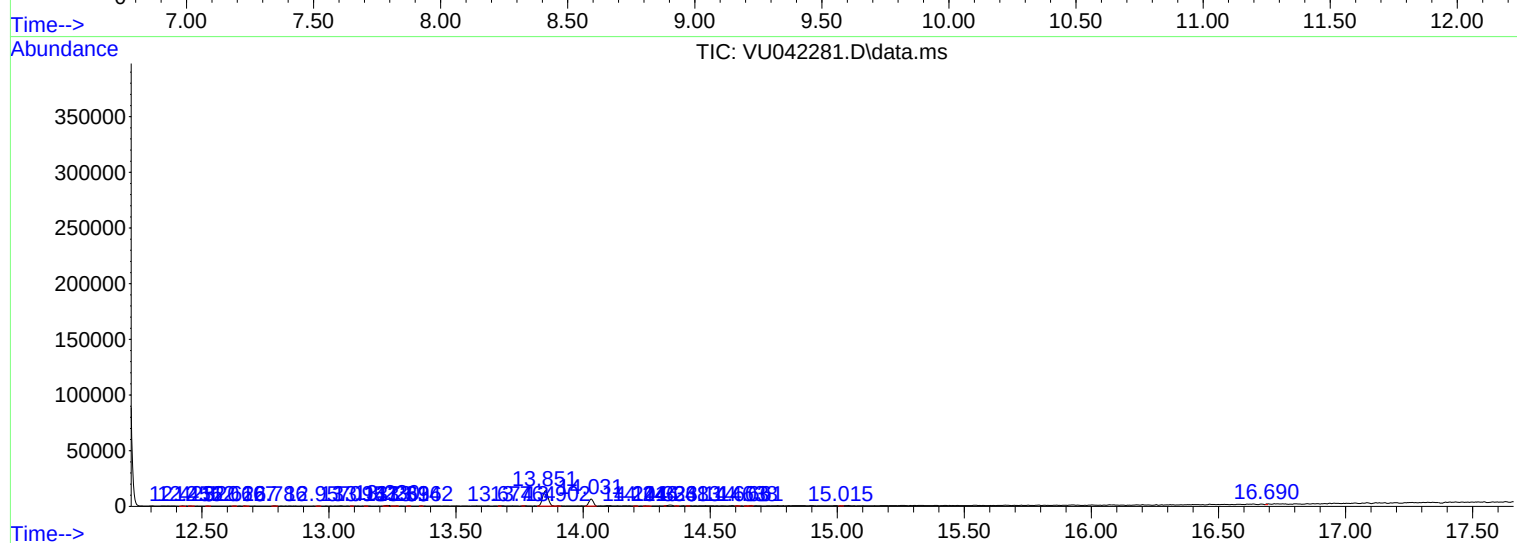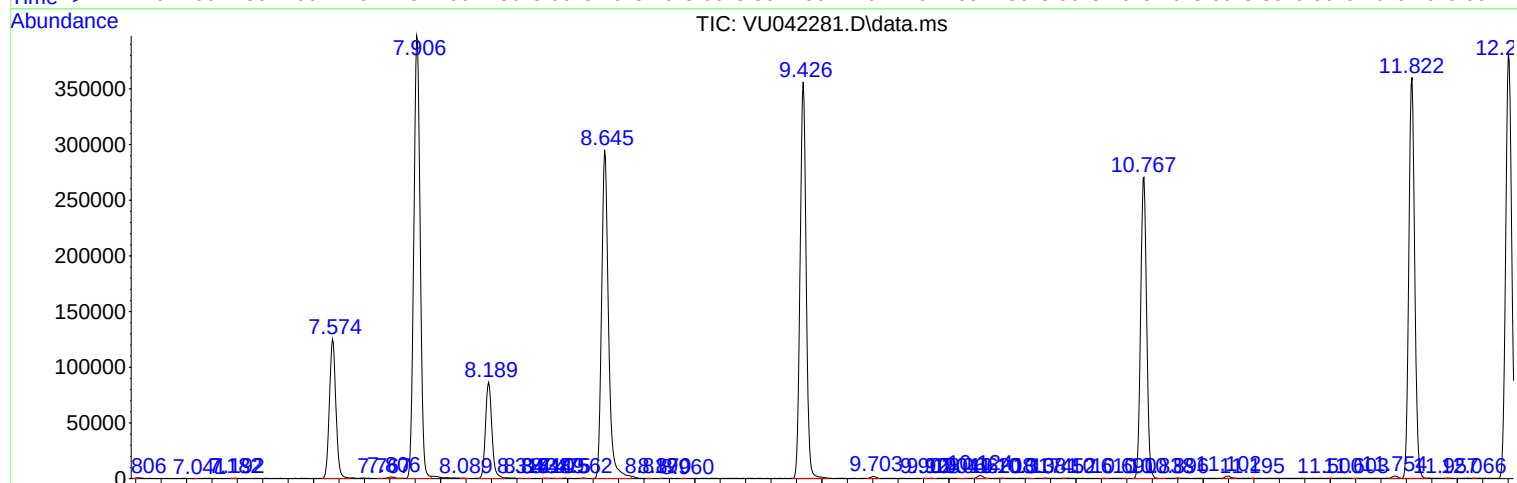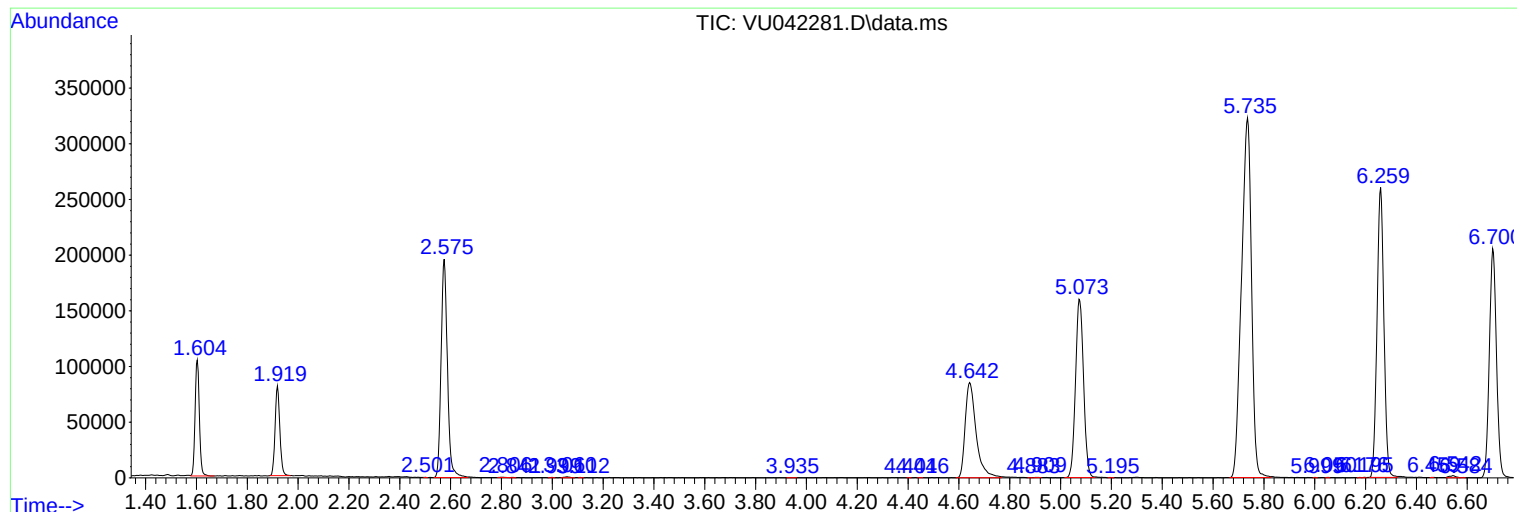

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020521\
Data File : VU042281.D
Acq On : 05 Feb 2021 16:22
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020521\
Data File : VU042281.D
Acq On : 05 Feb 2021 16:22
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
