
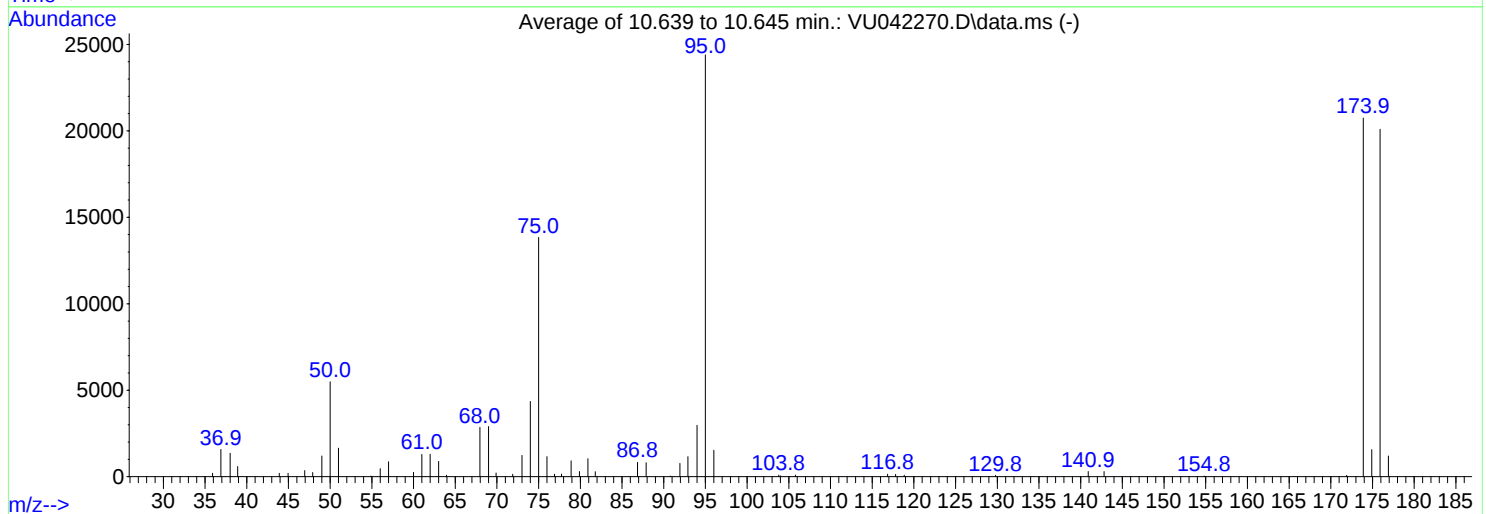


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020521\
 Data File : VU042270.D
 Acq On : 05 Feb 2021 08:52
 Operator : SY/MD
 Sample : BFB62
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB620

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020521WMA.M
 Title : VOC Analysis
 Last Update : Sat Feb 06 07:13:30 2021

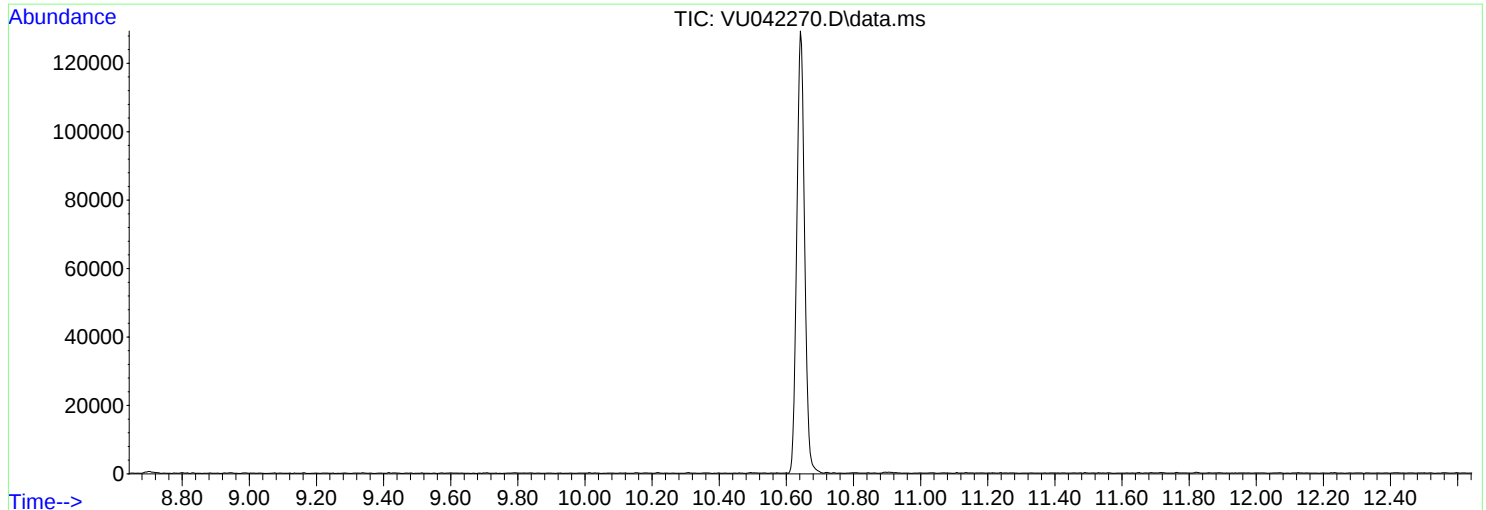

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	5487	PASS
75	95	30	80	56.7	13835	PASS
95	95	100	100	100.0	24400	PASS
96	95	5	9	6.3	1528	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.0	20744	PASS
175	174	5	9	7.5	1561	PASS
176	174	95	101	96.9	20091	PASS
177	176	5	9	5.9	1191	PASS

m/z	Abundance
35.90	213.0
36.90	1654.0
38.00	1313.0
38.90	560.0
43.90	452.0
44.90	188.0
46.90	341.0
47.90	237.0
49.00	1186.0
50.00	5472.0
51.00	1645.0
54.90	109.0
56.00	458.0
57.00	880.0
60.00	270.0
61.00	1241.0
62.00	1275.0
63.00	925.0
64.00	132.0
67.90	2849.0
69.00	2903.0
69.90	207.0
71.90	116.0
73.00	1150.0
74.00	4217.0
75.00	13482.0
76.00	1138.0
76.90	141.0
77.70	132.0
78.90	947.0
79.90	272.0
80.90	944.0
81.80	262.0
86.90	827.0
87.90	772.0
91.90	738.0
92.90	1129.0
94.00	2990.0
95.00	23560.0
96.00	1532.0
103.80	136.0
116.80	158.0
117.80	134.0
129.80	111.0
140.90	276.0
142.80	308.0
173.90	19336.0
174.90	1474.0
175.90	19280.0
176.90	1042.0

Instrument :
MSVOA_U
ClientSampleId :
BFB620

m/z	Abundance
35.90	197.0
36.90	1607.0
38.00	1415.0
38.90	599.0
43.90	441.0
44.90	199.0
47.00	361.0
47.90	252.0
49.00	1224.0
50.00	5658.0
51.00	1681.0
56.00	472.0
57.00	899.0
60.00	264.0
61.00	1327.0
62.00	1338.0
63.00	874.0
63.90	109.0
68.00	2938.0
69.00	2996.0
69.90	229.0
71.90	149.0
73.00	1299.0
74.00	4458.0
75.00	14308.0
76.00	1183.0
76.90	153.0
77.70	169.0
78.90	932.0
79.90	310.0
80.90	1079.0
81.80	301.0
86.90	843.0
87.90	813.0
92.00	783.0
92.90	1205.0
94.00	3074.0
95.00	25192.0
96.00	1538.0
103.80	146.0
105.80	124.0
116.90	140.0
117.80	136.0
118.90	117.0
129.80	112.0
140.90	313.0
142.80	298.0
171.90	105.0
173.90	21440.0
174.90	1603.0
175.90	20752.0
176.90	1244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB620

m/z	Abundance
35.90	187.0
36.90	1454.0
38.00	1330.0
38.90	579.0
43.90	404.0
45.00	211.0
47.00	352.0
47.90	221.0
49.00	1160.0
50.00	5330.0
51.00	1609.0
56.00	455.0
57.00	812.0
60.00	223.0
61.00	1300.0
62.00	1271.0
63.00	835.0
68.00	2761.0
69.00	2791.0
69.90	209.0
71.90	165.0
73.00	1243.0
74.00	4383.0
75.00	13714.0
76.00	1152.0
76.90	130.0
77.80	137.0
78.90	881.0
79.90	319.0
80.90	1079.0
81.80	289.0
86.80	805.0
87.90	817.0
90.80	106.0
92.00	770.0
92.90	1145.0
94.00	2844.0
95.00	24448.0
96.00	1514.0
104.00	146.0
105.80	146.0
116.90	113.0
117.80	124.0
118.80	138.0
140.90	308.0
142.80	274.0
154.80	105.0
171.90	116.0
173.90	21456.0
174.90	1607.0
175.90	20240.0
176.90	1287.0

Instrument :
MSVOA_U
ClientSampleId :
BFB620

m/z	Abundance
43.90	238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB620