
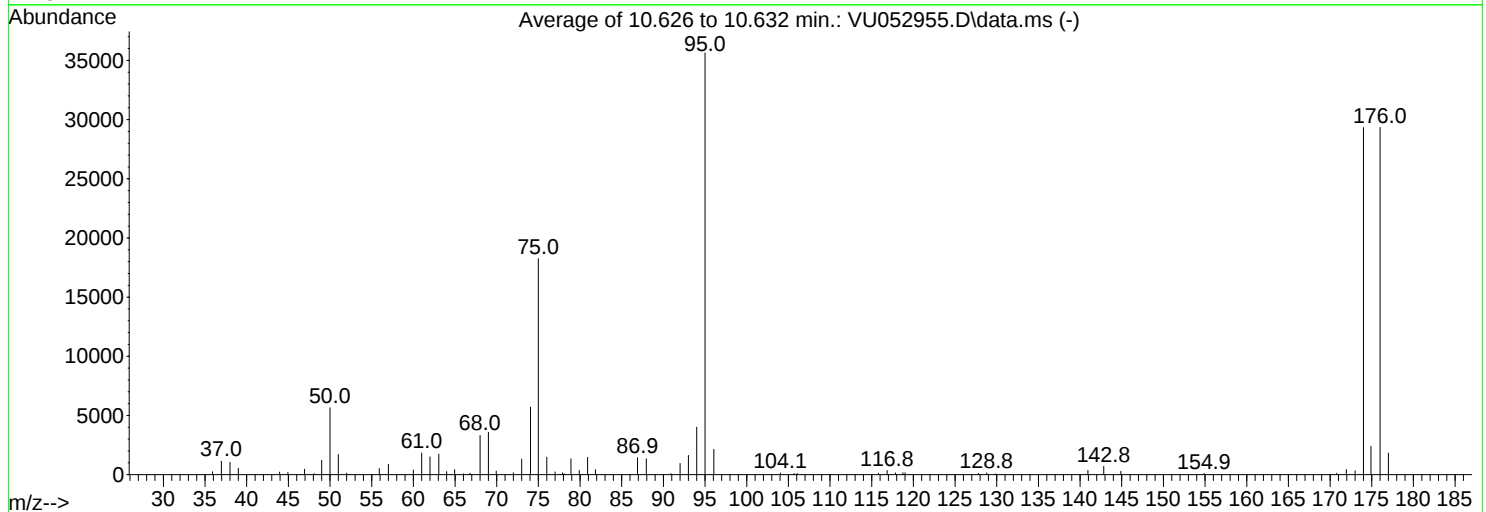


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020523\
 Data File : VU052955.D
 Acq On : 05 Feb 2023 14:00
 Operator : JC/MD
 Sample : BFB193
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB193

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sun Feb 05 21:58:05 2023

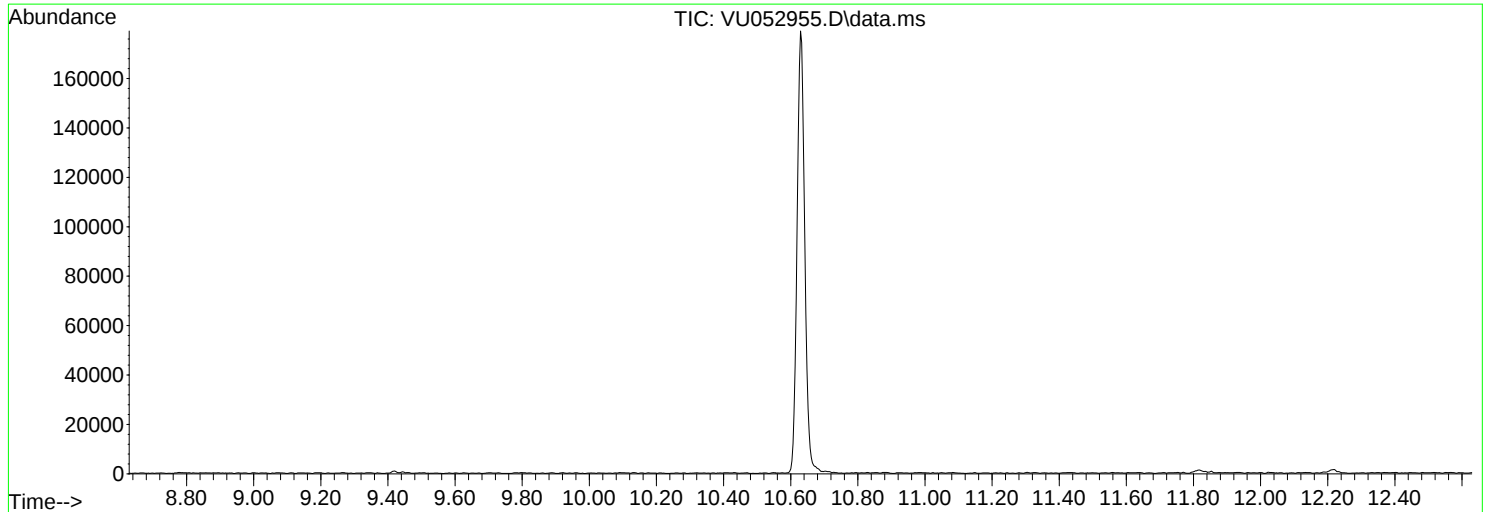

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	5658	PASS
75	95	30	80	51.2	18259	PASS
95	95	100	100	100.0	35640	PASS
96	95	5	9	6.0	2140	PASS
173	174	0.00	2	1.1	327	PASS
174	95	50	120	82.3	29323	PASS
175	174	5	9	8.2	2400	PASS
176	174	95	101	100.0	29336	PASS
177	176	5	9	6.2	1826	PASS

m/z	Abundance
43.90	324.0

Instrument :
MSVOA_U
ClientSampleId :
BFB193

m/z	Abundance
35.90	237.0
37.00	1127.0
38.00	1110.0
39.00	528.0
44.00	504.0
44.90	165.0
47.00	486.0
48.10	133.0
49.00	1097.0
50.00	5268.0
51.00	1660.0
52.00	135.0
55.90	492.0
57.00	899.0
60.00	410.0
61.00	1684.0
62.00	1560.0
63.10	1819.0
64.00	340.0
64.90	402.0
66.80	122.0
68.00	3432.0
69.00	3603.0
69.90	272.0
72.00	172.0
73.00	1308.0
74.00	5422.0
75.00	17472.0
76.00	1358.0
77.00	183.0
77.90	243.0
78.90	1322.0
79.90	328.0
80.90	1403.0
81.80	388.0
86.90	1307.0
88.00	1452.0
92.00	890.0
93.00	1574.0
94.00	3973.0
95.00	33944.0
96.00	2098.0
104.00	144.0
105.70	138.0
115.80	114.0
116.90	354.0
117.90	163.0
118.70	268.0
127.80	123.0
128.80	139.0
129.90	107.0
141.00	366.0
142.80	609.0
144.90	260.0
170.80	112.0
172.00	459.0
173.10	309.0
174.00	27752.0
174.90	2318.0
176.00	27192.0
177.00	1607.0

Instrument :
MSVOA_U
ClientSampleId :
BFB193

m/z	Abundance
35.90	249.0
36.90	1178.0
38.00	1027.0
39.00	562.0
44.00	562.0
44.90	211.0
47.00	483.0
49.00	1266.0
50.00	5873.0
51.00	1736.0
52.00	143.0
55.90	523.0
57.00	884.0
60.00	411.0
61.00	1897.0
62.00	1535.0
63.10	1765.0
64.00	254.0
65.00	458.0
66.00	109.0
66.80	126.0
68.00	3380.0
69.00	3654.0
69.90	294.0
72.00	160.0
73.00	1352.0
74.10	5902.0
75.00	19128.0
76.00	1543.0
77.00	242.0
77.90	213.0
78.90	1363.0
79.90	385.0
80.90	1524.0
81.80	458.0
86.90	1472.0
88.00	1362.0
90.90	122.0
92.00	938.0
93.00	1678.0
94.00	4215.0
95.00	37072.0
96.00	2194.0
104.00	142.0
105.70	141.0
106.10	128.0
115.80	118.0
116.90	351.0
117.90	143.0
118.80	237.0
119.00	243.0
127.80	115.0
128.80	172.0
129.90	101.0
140.90	380.0
142.90	723.0
144.90	286.0
154.90	138.0
170.80	120.0
171.90	441.0
173.00	316.0
174.00	30208.0
174.90	2496.0
176.00	30352.0
177.00	1921.0

Instrument :
MSVOA_U
ClientSampleId :
BFB193

m/z	Abundance
35.90	229.0
37.00	1095.0
38.00	970.0
39.00	524.0
44.00	565.0
45.00	203.0
46.90	421.0
48.10	102.0
49.00	1244.0
50.00	5832.0
51.00	1699.0
52.00	133.0
55.90	524.0
57.00	804.0
60.00	345.0
61.00	1890.0
62.00	1400.0
63.00	1601.0
63.90	181.0
65.00	454.0
66.00	117.0
66.80	109.0
68.00	3138.0
69.00	3475.0
70.00	311.0
72.00	176.0
73.00	1288.0
74.00	5777.0
75.00	18176.0
76.00	1514.0
77.00	268.0
78.10	203.0
78.90	1350.0
79.90	363.0
80.90	1457.0
81.90	416.0
86.90	1516.0
87.90	1212.0
90.90	160.0
92.00	1032.0
93.00	1606.0
94.00	3848.0
95.00	35904.0
96.10	2128.0
104.10	135.0
106.00	148.0
115.80	118.0
116.80	340.0
117.70	142.0
119.00	258.0
127.80	102.0
128.80	137.0
140.90	343.0
142.90	774.0
144.90	323.0
154.90	180.0
170.80	129.0
171.90	416.0
172.90	357.0
174.00	30008.0
174.90	2386.0
176.00	30464.0
177.00	1950.0

Instrument :
MSVOA_U
ClientSampleId :
BFB193