


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020524\
Data File : VU057801.D
Acq On : 05 Feb 2024 10:21
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Feb 07 04:06:29 2024

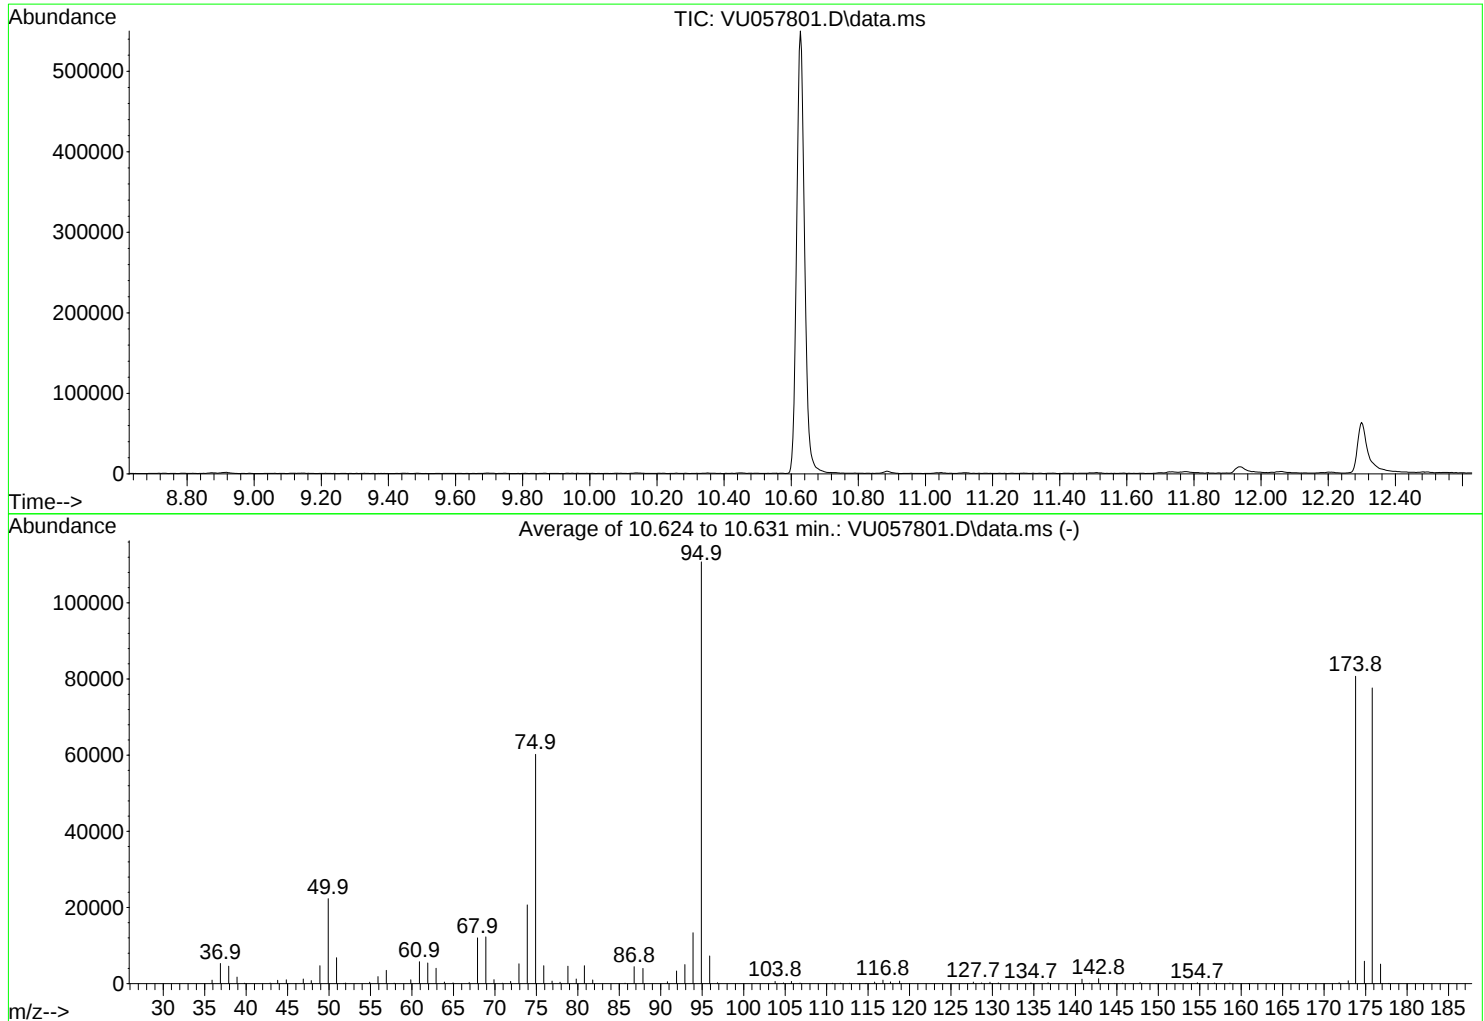

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	22307	PASS
75	95	30	60	54.4	60232	PASS
95	95	100	100	100.0	110787	PASS
96	95	5	9	6.6	7291	PASS
173	174	0.00	2	0.9	763	PASS
174	95	50	100	72.9	80739	PASS
175	174	5	9	7.3	5864	PASS
176	174	95	101	96.2	77659	PASS
177	176	5	9	6.6	5136	PASS