


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020619\
Data File : VU029354.D
Acq On : 06 Feb 2019 09:34
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U020519DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Feb 08 10:52:46 2019

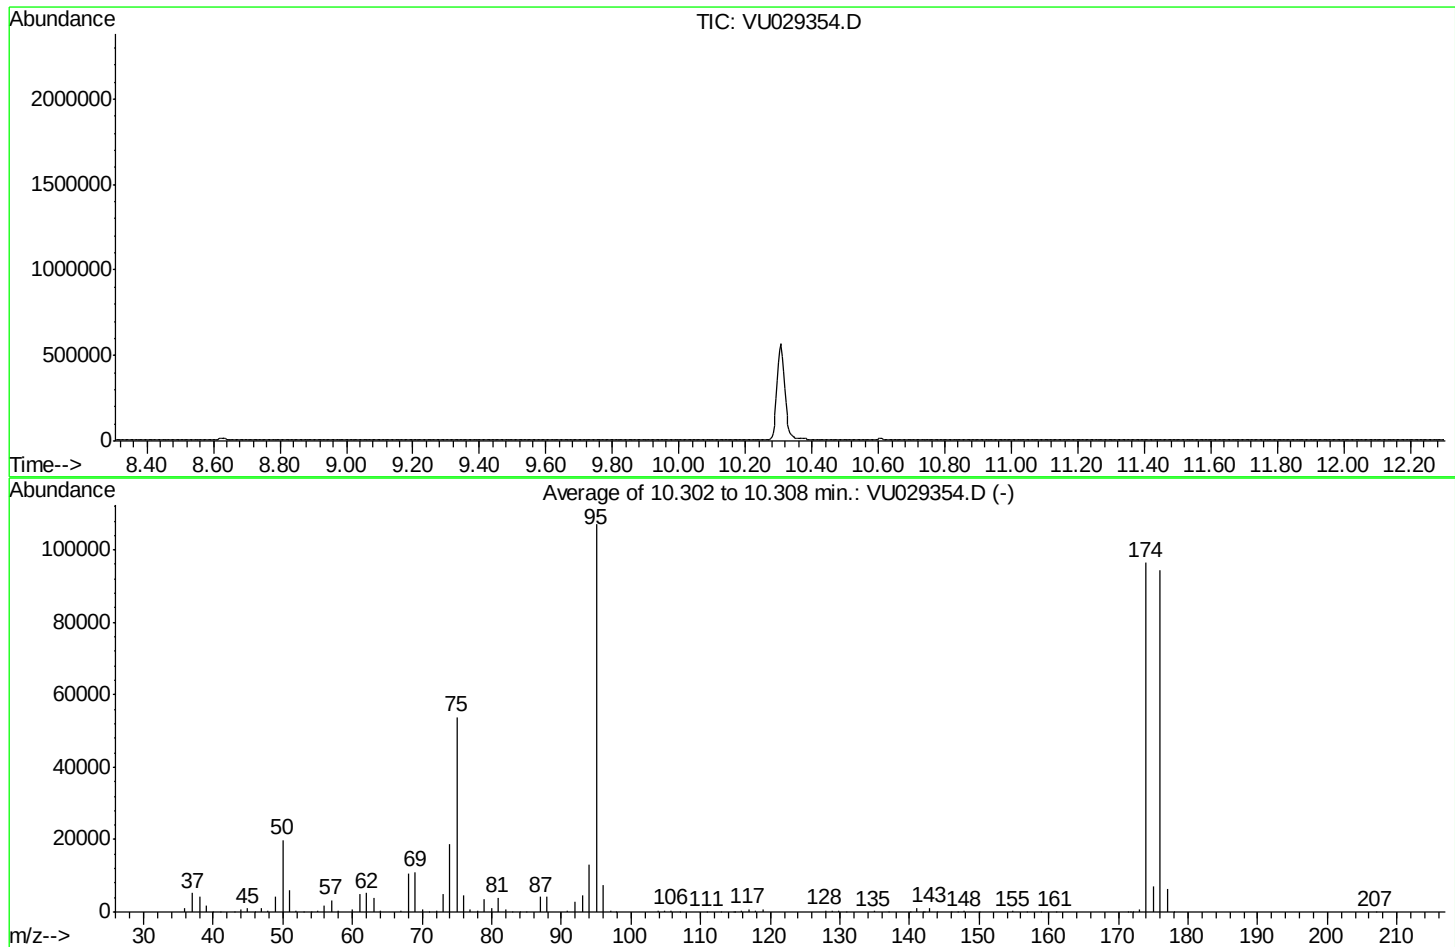

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	19832	PASS
75	95	30	60	50.3	53808	PASS
95	95	100	100	100.0	107056	PASS
96	95	5	9	7.0	7447	PASS
173	174	0.00	2	0.9	848	PASS
174	95	50	100	90.0	96400	PASS
175	174	5	9	7.3	7050	PASS
176	174	95	101	97.8	94317	PASS
177	176	5	9	6.6	6258	PASS