
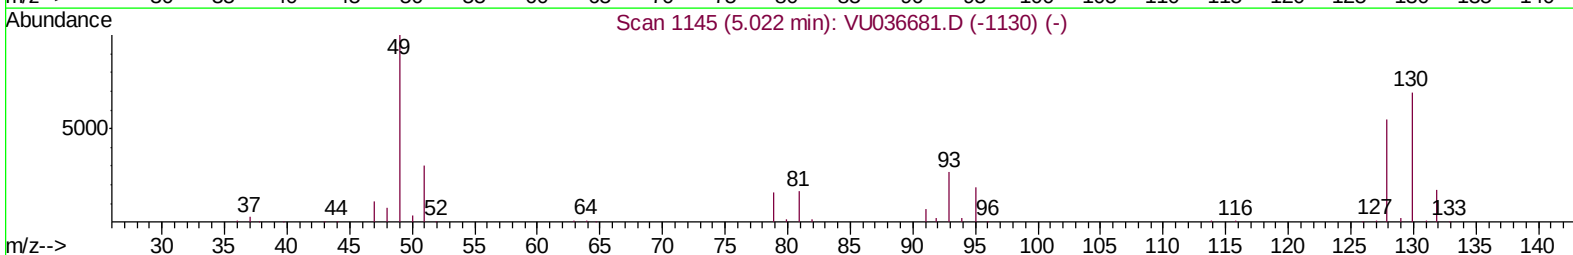
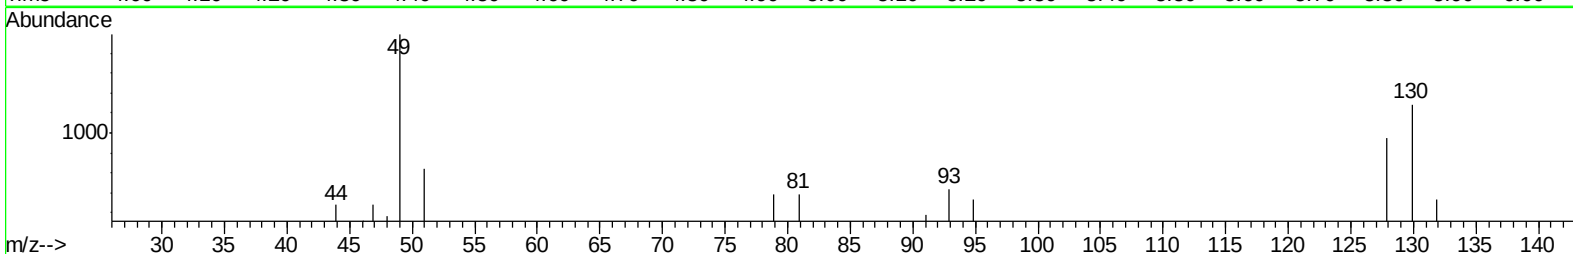


Data File : VU036687.D
Acq On : 06 Feb 2020 15:43
Operator : JC/MD
Sample : MDL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Feb 07 04:55:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 07 04:51:54 2020
Response via : Initial Calibration

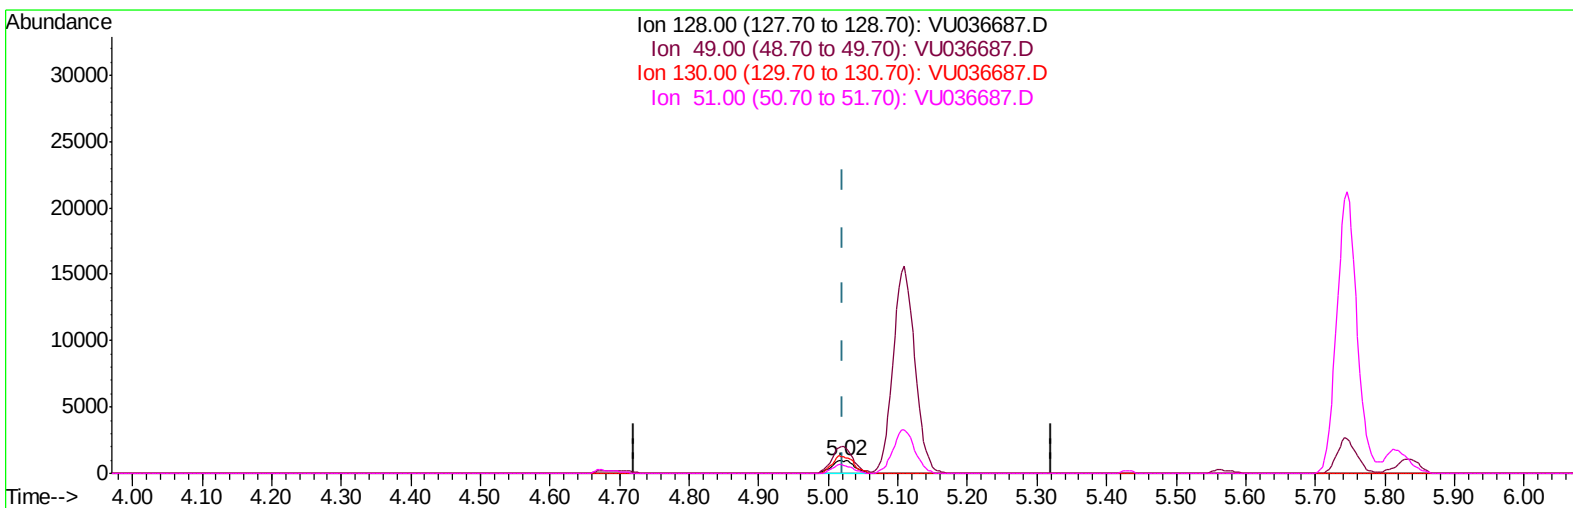

TIC: VU036687.D

(23) Bromochloromethane (T)

5.018min (-0.003) 2.34ug/L m

response 2206

Ion	Exp%	Act%
128.00	100	100
49.00	181.90	211.13
130.00	126.40	136.37
51.00	55.50	67.13#