
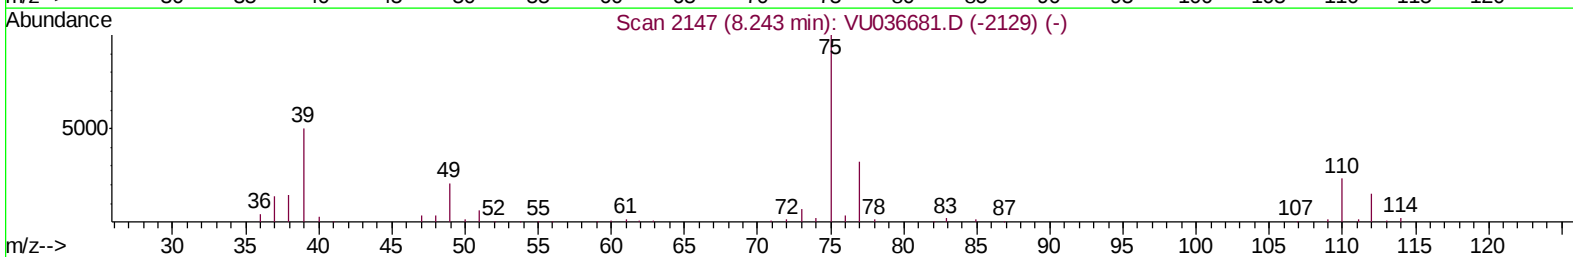
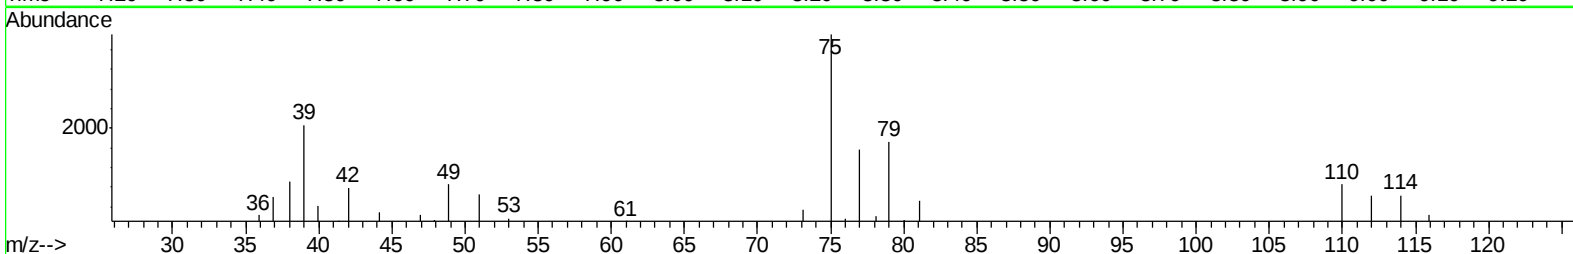


Data File : VU036687.D
Acq On : 06 Feb 2020 15:43
Operator : JC/MD
Sample : MDL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Feb 07 04:55:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 07 04:51:54 2020
Response via : Initial Calibration

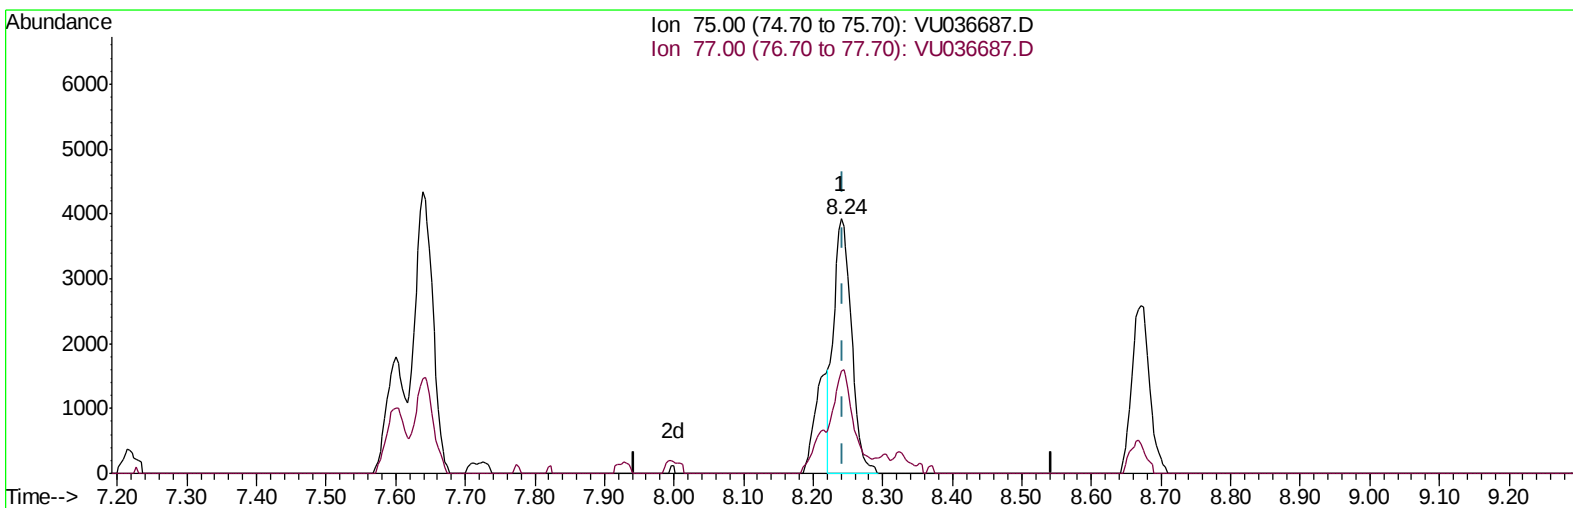

TIC: VU036687.D

(44) trans-1,3-Dichloropropene (T)

8.240min (-0.003) 2.42ug/L m

response 6944

Ion	Exp%	Act%
75.00	100	100
77.00	32.30	40.23
0.00	0.00	0.00
0.00	0.00	0.00