

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020620\
 Data File : VU036685.D
 Acq On : 06 Feb 2020 14:52
 Operator : JC/MD
 Sample : VU0206WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Quant Time: Feb 07 04:59:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 07 04:51:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	271985	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	256612	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.83	152	109676	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	92342	50.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.82%
7) Chloroethane-d5	1.93	69	84530	50.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.52%
11) 1,1-Dichloroethene-d2	2.59	63	127595	37.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.52%
21) 2-Butanone-d5	4.67	46	170831	110.39	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.39%
24) Chloroform-d	5.11	84	162066	49.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.74%
26) 1,2-Dichloroethane-d4	5.74	65	116676	51.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.92%
32) Benzene-d6	5.76	84	349999	51.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.76%
36) 1,2-Dichloropropane-d6	6.73	67	116482	52.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.02%
41) Toluene-d8	7.93	98	320242	51.83	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.66%
43) trans-1,3-Dichloropropene-	8.21	79	54578	50.90	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.80%
47) 2-Hexanone-d5	8.66	63	132710	103.83	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.83%
56) 1,1,2,2-Tetrachloroethane-	10.78	84	164861	49.95	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.90%
66) 1,2-Dichlorobenzene-d4	12.21	152	105694	53.04	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.08%


Target Compounds					Ovalue
13) Acetone	2.66	43	4775	2.905 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020620\
Data File : VU036685.D
Acq On : 06 Feb 2020 14:52
Operator : JC/MD
Sample : VU0206WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Time: Feb 07 04:59:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 07 04:51:54 2020
Response via : Initial Calibration

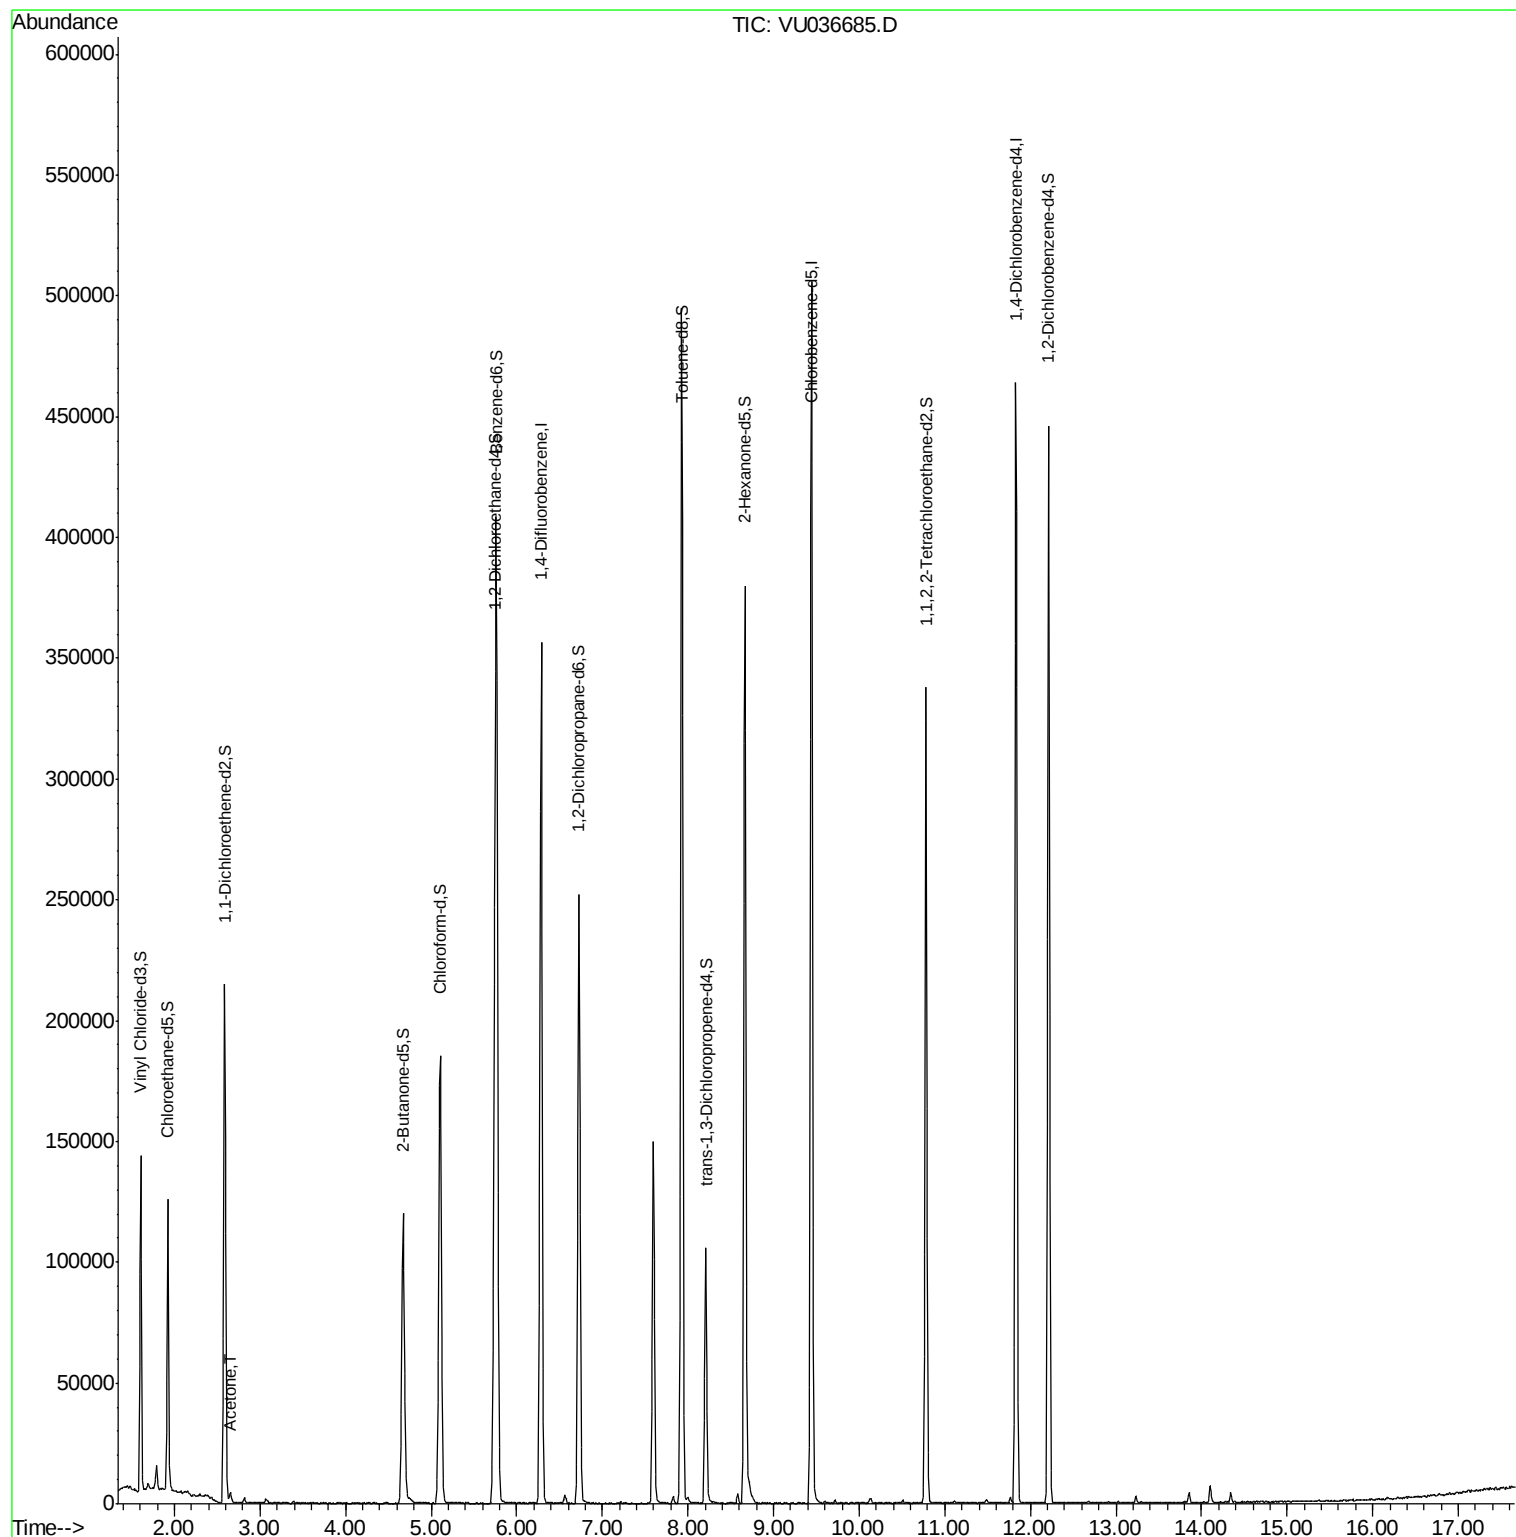

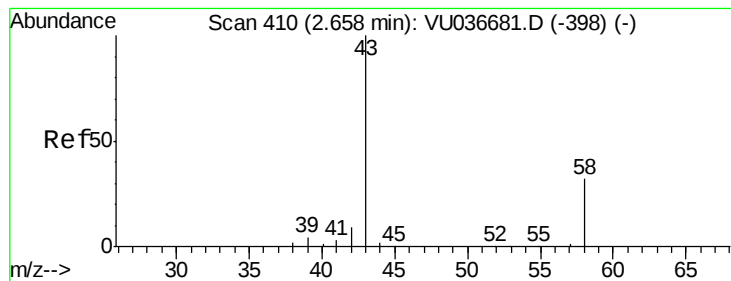

#13
 Acetone
 Concen: 2.905 ug/L
 RT: 2.66 min Scan# 409
 Delta R.T. -0.00 min
 Lab File: VU036685.D
 Acq: 06 Feb 2020 14:52

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Tot Ion: 43 Resp: 4775
 Ion Ratio Lower Upper
 43 100
 58 27.9 0.0 64.0

