

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020620\
 Data File : VU036686.D
 Acq On : 06 Feb 2020 15:15
 Operator : JC/MD
 Sample : VU0206WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK102

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	97	rBV	124541	134635	13.65%	1.744%
2	1.932	176	184	197	rVB	108730	144343	14.64%	1.869%
3	2.594	378	390	405	rBV	194215	319493	32.40%	4.137%
4	3.083	535	542	553	rVB3	1935	2952	0.30%	0.038%
5	3.231	576	588	598	rVB2	1183	2460	0.25%	0.032%
6	3.369	625	631	633	rBV	247	189	0.02%	0.002%
7	3.391	633	638	641	rBV2	378	406	0.04%	0.005%
8	3.475	662	664	665	rBV2	109	44	0.00%	0.001%
9	3.620	706	709	712	rBV2	276	180	0.02%	0.002%
10	3.732	742	744	746	rBV2	138	79	0.01%	0.001%
11	3.896	792	795	797	rVB	92	51	0.01%	0.001%
12	4.025	832	835	842	rBV	99	94	0.01%	0.001%
13	4.057	842	845	848	rVB	116	73	0.01%	0.001%
14	4.102	857	859	862	rBV	152	90	0.01%	0.001%
15	4.237	899	901	902	rBV	150	44	0.00%	0.001%
16	4.298	917	920	924	rBV	66	67	0.01%	0.001%
17	4.378	942	945	946	rBV	112	63	0.01%	0.001%
18	4.417	954	957	959	rBV	72	45	0.00%	0.001%
19	4.558	994	1001	1004	rBV	108	117	0.01%	0.002%
20	4.607	1011	1016	1019	rBV	103	115	0.01%	0.001%
21	4.677	1023	1038	1061	rBV	114563	264462	26.82%	3.425%
22	5.112	1155	1173	1192	rBV	175301	375928	38.12%	4.868%
23	5.333	1237	1242	1249	rVB3	605	972	0.10%	0.013%
24	5.423	1267	1270	1276	rVB3	519	370	0.04%	0.005%
25	5.481	1286	1288	1291	rVB	131	72	0.01%	0.001%
26	5.501	1291	1294	1298	rVB	113	100	0.01%	0.001%
27	5.539	1303	1306	1308	rBV	97	74	0.01%	0.001%
28	5.591	1319	1322	1324	rBV	134	85	0.01%	0.001%
29	5.603	1324	1326	1329	rVV	60	38	0.00%	0.000%
30	5.690	1348	1353	1355	rBV	99	96	0.01%	0.001%
31	5.767	1355	1377	1402	rBV2	377518	986105	100.00%	12.770%
32	6.018	1453	1455	1457	rVB	266	96	0.01%	0.001%
33	6.031	1457	1459	1464	rBV2	193	147	0.01%	0.002%
34	6.076	1470	1473	1476	rVB2	354	259	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020620\
 Data File : VU036686.D
 Acq On : 06 Feb 2020 15:15
 Operator : JC/MD
 Sample : VU0206WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK102

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

35	6.121	1479	1487	1489	rBV2	244	229	0.02%	0.003%
36	6.134	1489	1491	1492	rBV	133	49	0.00%	0.001%
37	6.195	1505	1510	1511	rBV	257	201	0.02%	0.003%
38	6.288	1524	1539	1559	rBV	323867	607705	61.63%	7.870%
39	6.526	1610	1613	1618	rBV2	265	172	0.02%	0.002%
40	6.565	1618	1625	1634	rVV5	2135	3729	0.38%	0.048%
41	6.600	1634	1636	1639	rVB	252	125	0.01%	0.002%
42	6.642	1645	1649	1653	rBV	244	246	0.02%	0.003%
43	6.732	1662	1677	1694	rBV	237866	457696	46.41%	5.927%
44	6.873	1717	1721	1724	rVB3	295	187	0.02%	0.002%
45	6.896	1724	1728	1731	rVB	76	55	0.01%	0.001%
46	6.912	1731	1733	1739	rBV	100	90	0.01%	0.001%
47	6.941	1740	1742	1746	rVB	96	66	0.01%	0.001%
48	6.967	1746	1750	1753	rBV	88	66	0.01%	0.001%
49	7.089	1780	1788	1790	rBV	116	145	0.01%	0.002%
50	7.182	1814	1817	1820	rBV	97	70	0.01%	0.001%
51	7.221	1822	1829	1837	rVV3	482	746	0.08%	0.010%
52	7.346	1865	1868	1876	rBV	100	98	0.01%	0.001%
53	7.475	1905	1908	1911	rBV	61	40	0.00%	0.001%
54	7.510	1914	1919	1922	rBV	167	159	0.02%	0.002%
55	7.555	1930	1933	1935	rBV	151	79	0.01%	0.001%
56	7.600	1935	1947	1967	rBV	140398	242447	24.59%	3.140%
57	7.758	1990	1996	1999	rBV2	267	222	0.02%	0.003%
58	7.803	2006	2010	2011	rBV	165	106	0.01%	0.001%
59	7.832	2013	2019	2029	rVB4	1606	2156	0.22%	0.028%
60	7.931	2036	2050	2066	rBV	459586	782524	79.36%	10.134%
61	8.156	2117	2120	2121	rBV	168	84	0.01%	0.001%
62	8.211	2125	2137	2158	rBV	96811	164227	16.65%	2.127%
63	8.465	2212	2216	2221	rBV	146	146	0.01%	0.002%
64	8.494	2221	2225	2229	rBV2	353	445	0.05%	0.006%
65	8.529	2233	2236	2238	rBV	87	67	0.01%	0.001%
66	8.581	2243	2252	2260	rBV5	3362	5120	0.52%	0.066%
67	8.668	2264	2279	2319	rBV	348485	617652	62.64%	7.998%
68	8.822	2324	2327	2330	rBV	264	146	0.01%	0.002%
69	8.954	2364	2368	2370	rBV2	143	127	0.01%	0.002%
70	9.192	2438	2442	2448	rBV	511	592	0.06%	0.008%
71	9.352	2490	2492	2494	rBV	147	63	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU020620\
 Data File : VU036686.D
 Acq On : 06 Feb 2020 15:15
 Operator : JC/MD
 Sample : VU0206WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK102

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis

72	9.372	2495	2498	2502	rVB2	215	144	0.01%	0.002%
73	9.446	2508	2521	2544	rBV	453296	750425	76.10%	9.718%
74	9.600	2561	2569	2575	rBV2	690	876	0.09%	0.011%
75	9.629	2575	2578	2581	rBV	194	151	0.02%	0.002%
76	9.722	2601	2607	2614	rVB3	923	1214	0.12%	0.016%
77	9.774	2621	2623	2627	rVB2	246	187	0.02%	0.002%
78	9.796	2627	2630	2633	rVB	158	97	0.01%	0.001%
79	9.815	2633	2636	2640	rBV	266	180	0.02%	0.002%
80	9.896	2658	2661	2665	rVB	181	143	0.01%	0.002%
81	10.008	2693	2696	2697	rBV	103	63	0.01%	0.001%
82	10.076	2714	2717	2719	rBV	108	75	0.01%	0.001%
83	10.095	2721	2723	2724	rBV	125	33	0.00%	0.000%
84	10.134	2727	2735	2736	rBV2	982	963	0.10%	0.012%
85	10.452	2831	2834	2837	rBV	181	136	0.01%	0.002%
86	10.507	2847	2851	2852	rBV	404	279	0.03%	0.004%
87	10.629	2888	2889	2890	rBV	129	34	0.00%	0.000%
88	10.661	2896	2899	2900	rBV	167	77	0.01%	0.001%
89	10.783	2924	2937	2957	rBV	315436	509100	51.63%	6.593%
90	11.114	3032	3040	3046	rVB2	532	675	0.07%	0.009%
91	11.452	3143	3145	3148	rBV	181	76	0.01%	0.001%
92	11.494	3151	3158	3167	rVB2	820	1138	0.12%	0.015%
93	11.767	3238	3243	3249	rBV	1451	1542	0.16%	0.020%
94	11.835	3251	3264	3280	rVB	417032	669587	67.90%	8.671%
95	12.214	3369	3382	3397	rBV	409617	661373	67.07%	8.565%
96	12.478	3461	3464	3468	rVB	277	207	0.02%	0.003%
97	12.500	3468	3471	3476	rBV	274	227	0.02%	0.003%
98	12.909	3595	3598	3602	rBV2	299	185	0.02%	0.002%
99	13.012	3628	3630	3634	rBV2	263	147	0.01%	0.002%
100	14.175	3989	3992	3996	rBV	392	344	0.03%	0.004%


Sum of corrected areas: 7722099

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU020620\
Data File : VU036686.D
Acq On : 06 Feb 2020 15:15
Operator : JC/MD
Sample : VU0206WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK102

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

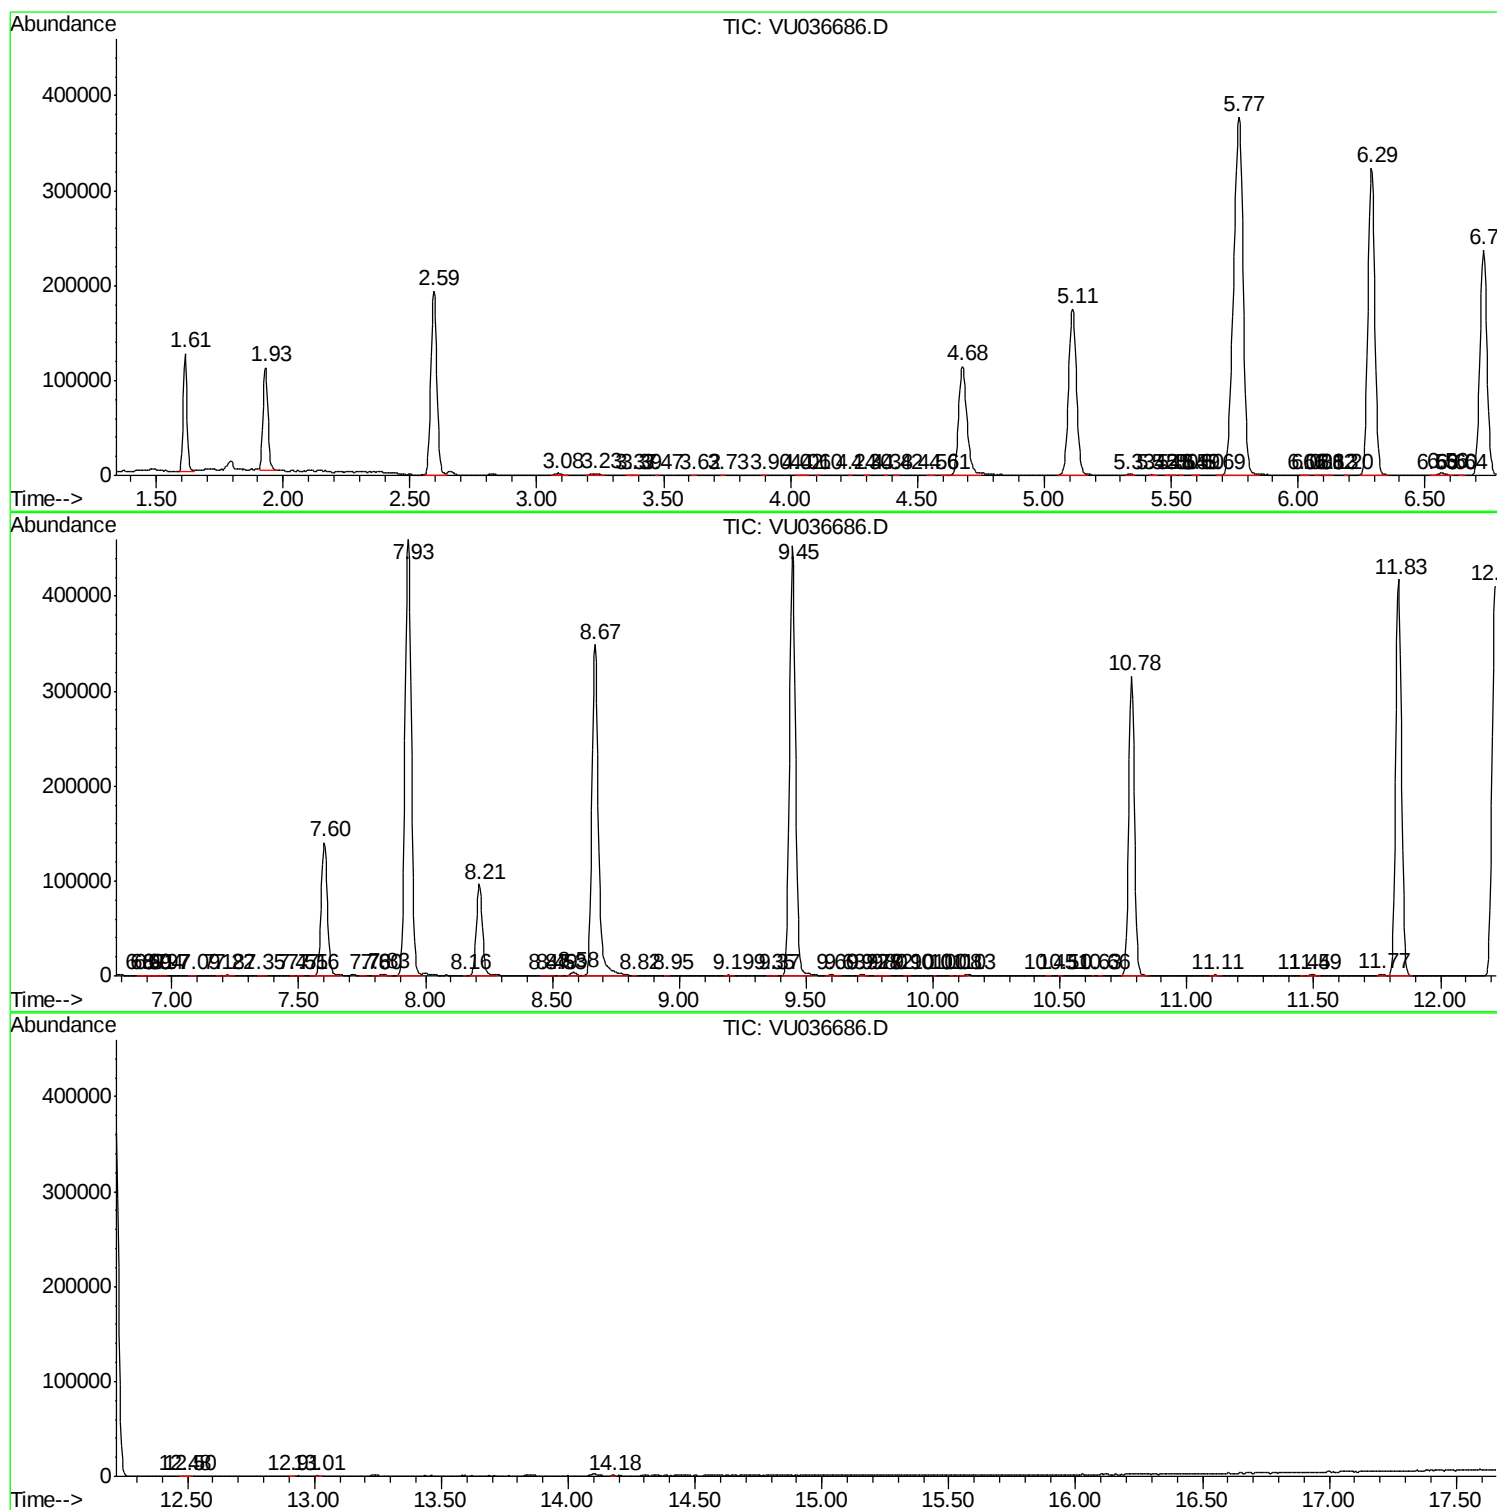

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU020620\
Data File : VU036686.D
Acq On : 06 Feb 2020 15:15
Operator : JC/MD
Sample : VU0206WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK102

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU020620\
Data File : VU036686.D
Acq On : 06 Feb 2020 15:15
Operator : JC/MD
Sample : VU0206WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK102

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc