


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU020620\
 Data File : VU036678.D
 Acq On : 06 Feb 2020 10:59
 Operator : JC/MD
 Sample : BFB48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB101

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM020620W.M
 Title : VOC Analysis
 Last Update : Fri Feb 07 04:51:54 2020

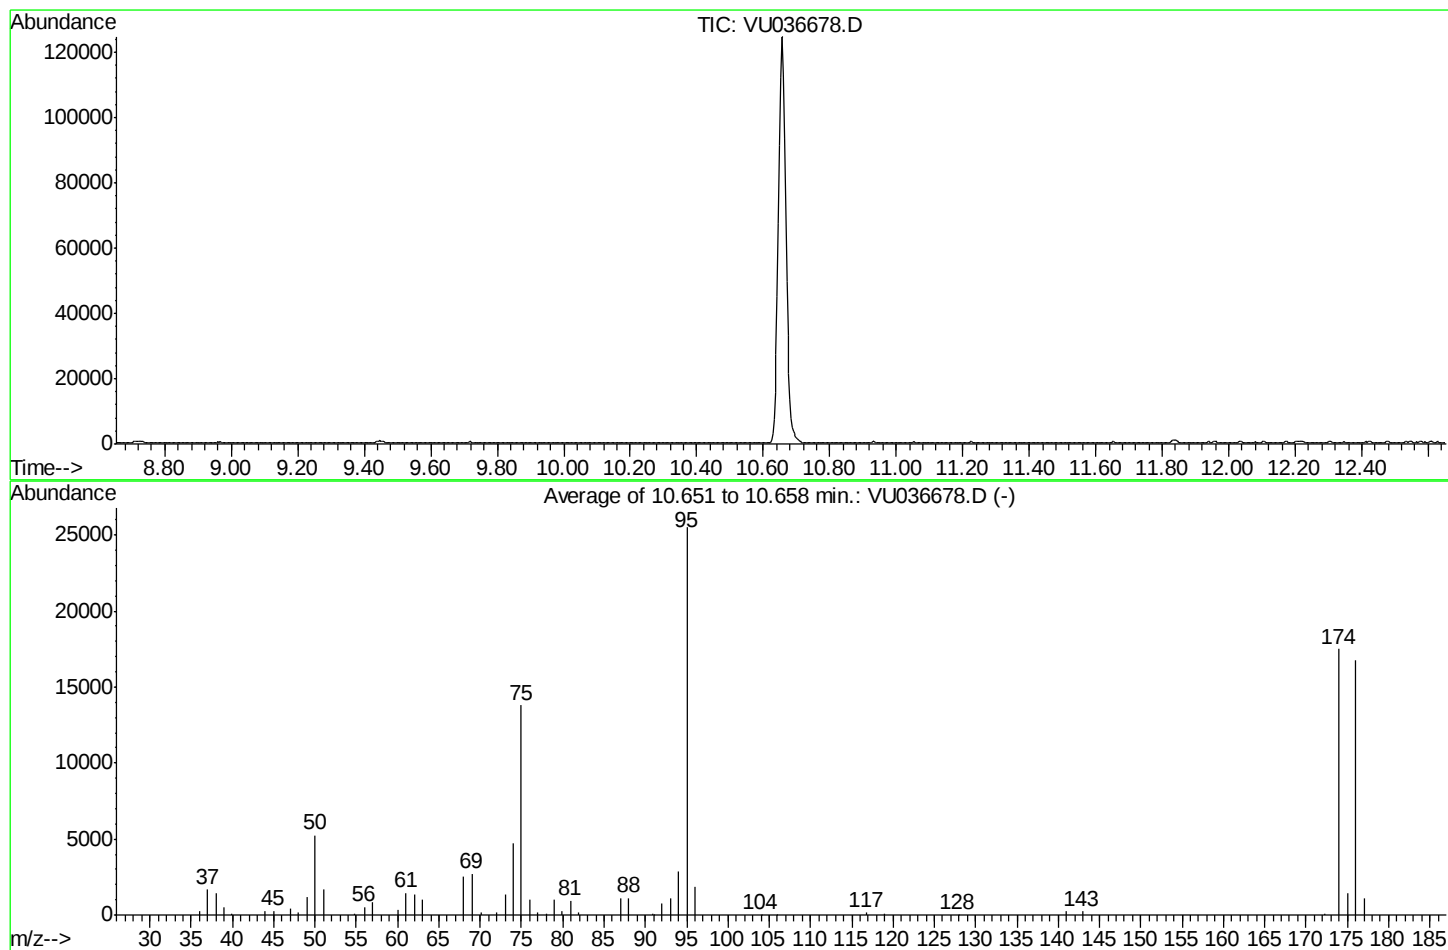

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	5261	PASS
75	95	30	80	54.1	13800	PASS
95	95	100	100	100.0	25512	PASS
96	95	5	9	7.2	1828	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.6	17503	PASS
175	174	5	9	8.0	1394	PASS
176	174	95	101	95.9	16790	PASS
177	176	5	9	6.5	1086	PASS

m/z	Abundance
35.00	298.0
37.00	1688.0
38.00	1263.0
39.00	459.0
43.00	532.0
45.00	269.0
47.00	321.0
47.00	166.0
49.00	1102.0
50.00	4989.0
51.00	1608.0
54.80	115.0
56.00	491.0
57.00	860.0
60.00	272.0
61.00	1450.0
62.00	1296.0
63.00	929.0
68.00	2343.0
69.00	2642.0
70.00	222.0
72.10	135.0
73.10	1248.0
74.00	4380.0
75.00	13033.0
76.00	916.0
76.00	120.0
78.00	150.0
79.00	882.0
79.00	248.0
80.00	929.0
81.00	208.0
87.00	1009.0
88.00	1067.0
90.00	123.0
92.00	624.0
93.00	1022.0
94.00	2656.0
95.00	24120.0
96.00	1764.0
116.80	143.0
118.00	121.0
140.00	228.0
143.00	227.0
174.00	15693.0
175.00	1310.0
176.00	15516.0
177.00	1031.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
35.00	305.0
37.00	1743.0
38.00	1483.0
39.00	561.0
39.00	107.0
43.00	575.0
45.00	286.0
47.00	417.0
47.00	169.0
49.00	1232.0
50.00	5415.0
51.00	1792.0
54.00	109.0
56.00	553.0
57.00	870.0
60.00	336.0
61.00	1529.0
62.00	1375.0
63.00	1051.0
68.00	2622.0
69.00	2787.0
70.10	219.0
72.10	164.0
73.10	1437.0
74.00	4934.0
75.00	14205.0
76.00	1011.0
76.00	148.0
78.00	132.0
79.00	1028.0
79.00	245.0
80.00	974.0
81.00	206.0
87.00	1138.0
88.00	1131.0
91.10	127.0
92.00	809.0
93.00	1116.0
94.10	2972.0
95.00	26528.0
96.00	1871.0
104.00	103.0
116.80	141.0
118.90	121.0
127.90	110.0
140.90	249.0
142.90	256.0
172.30	109.0
174.00	18080.0
175.00	1452.0
176.00	17208.0
177.00	1119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
36.00	279.0
37.00	1578.0
38.00	1453.0
39.00	568.0
39.90	102.0
43.90	585.0
44.90	278.0
47.00	455.0
48.00	162.0
49.00	1292.0
50.00	5379.0
51.00	1769.0
54.90	104.0
56.00	555.0
57.00	805.0
60.00	338.0
61.00	1443.0
62.00	1300.0
63.00	1064.0
68.00	2725.0
69.00	2723.0
70.00	194.0
72.00	189.0
73.10	1454.0
74.00	4831.0
75.00	14163.0
76.10	1108.0
77.00	157.0
78.90	1038.0
80.00	265.0
80.90	966.0
81.90	185.0
87.00	1146.0
88.00	1149.0
90.90	123.0
92.00	869.0
93.00	1107.0
94.10	3084.0
95.00	25888.0
96.00	1851.0
105.90	104.0
116.80	136.0
118.90	119.0
141.00	238.0
142.90	260.0
172.30	109.0
174.00	18736.0
175.00	1422.0
176.00	17648.0
177.00	1108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
44.00	338.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101