

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052980.D
 Acq On : 06 Feb 2023 15:05
 Operator : JC/MD
 Sample : 01444-05 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	95	rVB	82363	94012	16.45%	1.757%
2	1.913	169	178	193	rVB	72457	93729	16.40%	1.752%
3	2.565	369	381	396	rBV	134349	224473	39.27%	4.196%
4	3.044	519	530	542	rVB2	8848	16479	2.88%	0.308%
5	3.183	559	573	585	rBV2	6974	14696	2.57%	0.275%
6	3.356	613	627	637	rBV4	5395	9986	1.75%	0.187%
7	4.658	1009	1032	1074	rBV4	107738	379127	66.33%	7.087%
8	5.060	1141	1157	1179	rBV	113467	250238	43.78%	4.678%
9	5.723	1341	1363	1391	rBV2	214722	555377	97.17%	10.381%
10	6.247	1510	1526	1543	rBV	187843	358117	62.66%	6.694%
11	6.539	1602	1617	1638	rBV2	303790	571564	100.00%	10.684%
12	6.687	1650	1663	1681	rVB	133762	259991	45.49%	4.860%
13	7.562	1923	1935	1950	rBV	56105	99327	17.38%	1.857%
14	7.893	2025	2038	2055	rBV	245716	430354	75.29%	8.044%
15	8.176	2114	2126	2145	rBV	35583	60317	10.55%	1.127%
16	8.549	2230	2242	2255	rBV	60085	99866	17.47%	1.867%
17	8.633	2256	2268	2298	rBV2	232567	485619	84.96%	9.077%
18	9.414	2496	2511	2533	rBV	272759	451500	78.99%	8.440%
19	10.751	2913	2927	2943	rBV	101421	163854	28.67%	3.063%
20	11.809	3242	3256	3278	rBV	233380	372395	65.15%	6.961%
21	12.189	3361	3374	3393	rBV	219673	358754	62.77%	6.706%




Sum of corrected areas: 5349775

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052980.D
Acq On : 06 Feb 2023 15:05
Operator : JC/MD
Sample : 01444-05 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

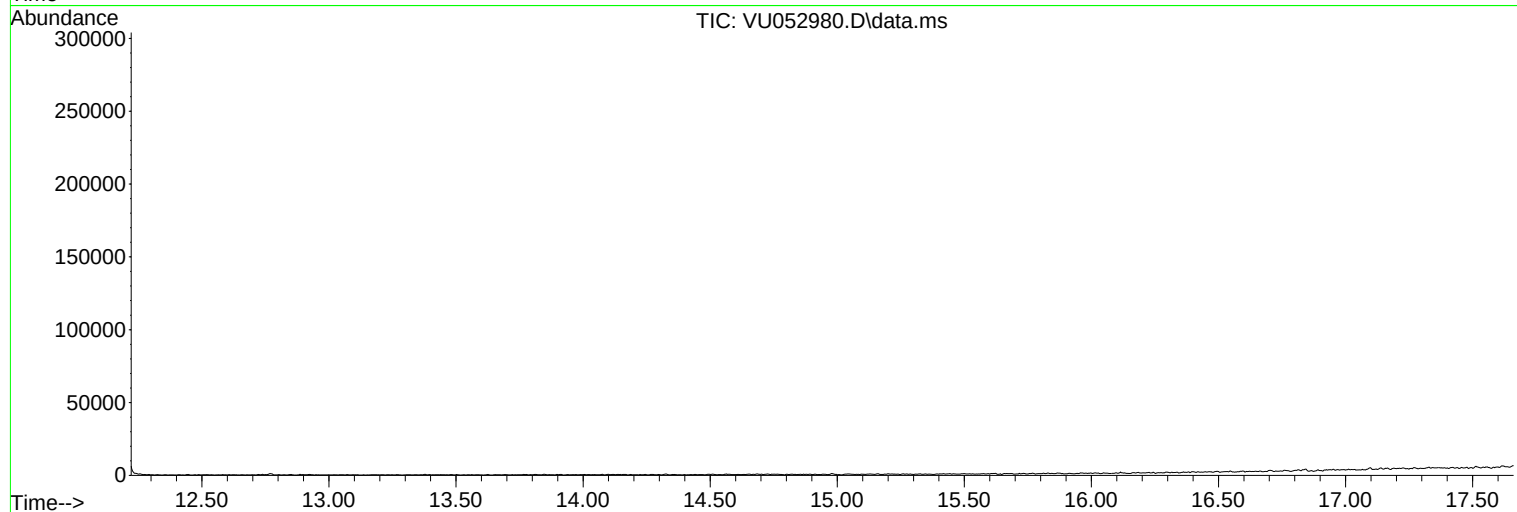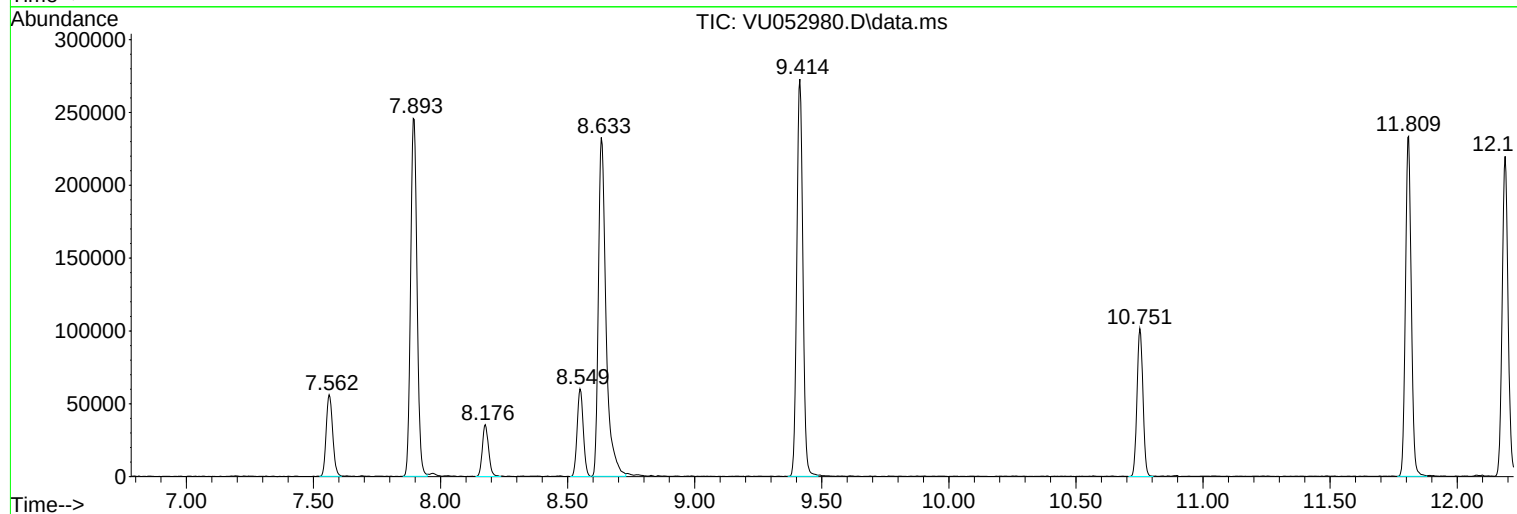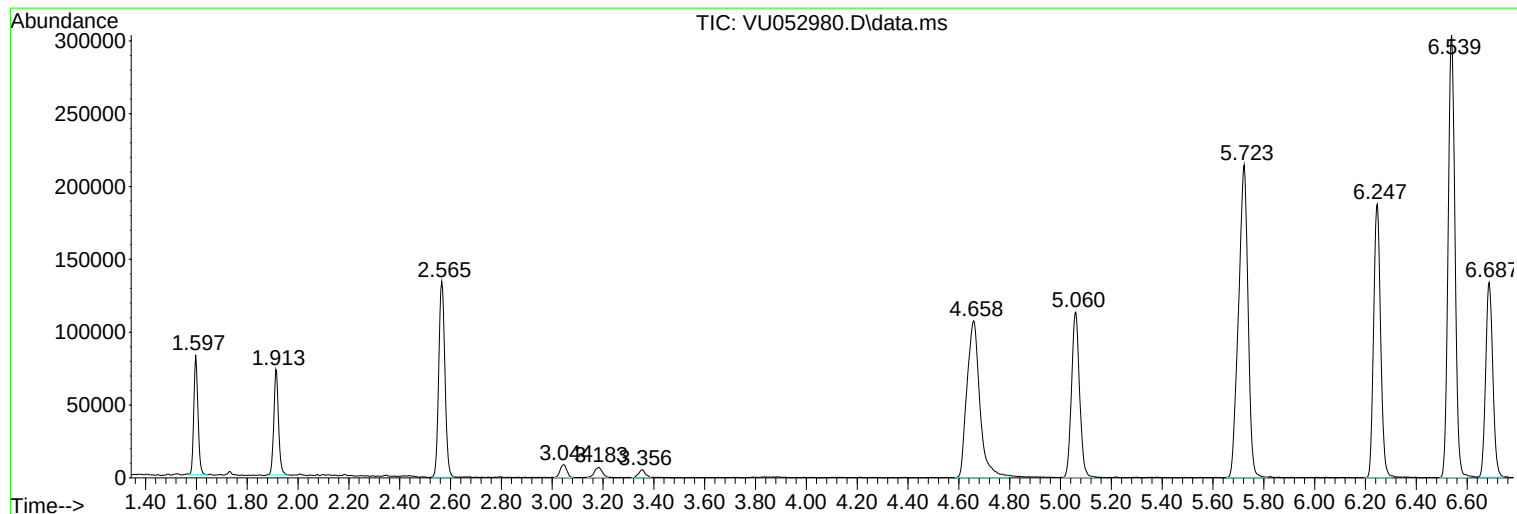

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052980.D
Acq On : 06 Feb 2023 15:05
Operator : JC/MD
Sample : 01444-05 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052980.D
Acq On : 06 Feb 2023 15:05
Operator : JC/MD
Sample : 01444-05 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc