

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052981.D
 Acq On : 06 Feb 2023 15:29
 Operator : JC/MD
 Sample : VIBLK145
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK145

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rVB	72099	85704	15.26%	1.915%
2	1.912	169	178	197	rVB	68768	91596	16.31%	2.046%
3	2.565	369	381	397	rBV	136297	224167	39.93%	5.008%
4	3.041	519	529	543	rBV4	8984	16804	2.99%	0.375%
5	4.645	1012	1028	1073	rBV	53094	203038	36.16%	4.536%
6	5.057	1141	1156	1181	rBV2	114776	252866	45.04%	5.649%
7	5.723	1342	1363	1386	rBV2	216062	561450	100.00%	12.543%
8	6.247	1512	1526	1544	rBV	183074	346490	61.71%	7.741%
9	6.539	1606	1617	1626	rBV8	3774	6845	1.22%	0.153%
10	6.687	1649	1663	1685	rBV	132609	264965	47.19%	5.919%
11	7.562	1920	1935	1952	rBV3	56039	99556	17.73%	2.224%
12	7.896	2026	2039	2059	rBV	247568	431547	76.86%	9.641%
13	8.176	2116	2126	2141	rBV	35538	60070	10.70%	1.342%
14	8.549	2232	2242	2253	rVB2	18484	29950	5.33%	0.669%
15	8.632	2253	2268	2295	rBV3	227235	485417	86.46%	10.844%
16	9.414	2498	2511	2530	rBV	261258	429432	76.49%	9.594%
17	10.751	2916	2927	2950	rVB	104824	169989	30.28%	3.798%
18	11.806	3244	3255	3271	rBV	222309	356156	63.44%	7.957%
19	12.189	3362	3374	3392	rBV	223697	360214	64.16%	8.047%




Sum of corrected areas: 4476256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052981.D
Acq On : 06 Feb 2023 15:29
Operator : JC/MD
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

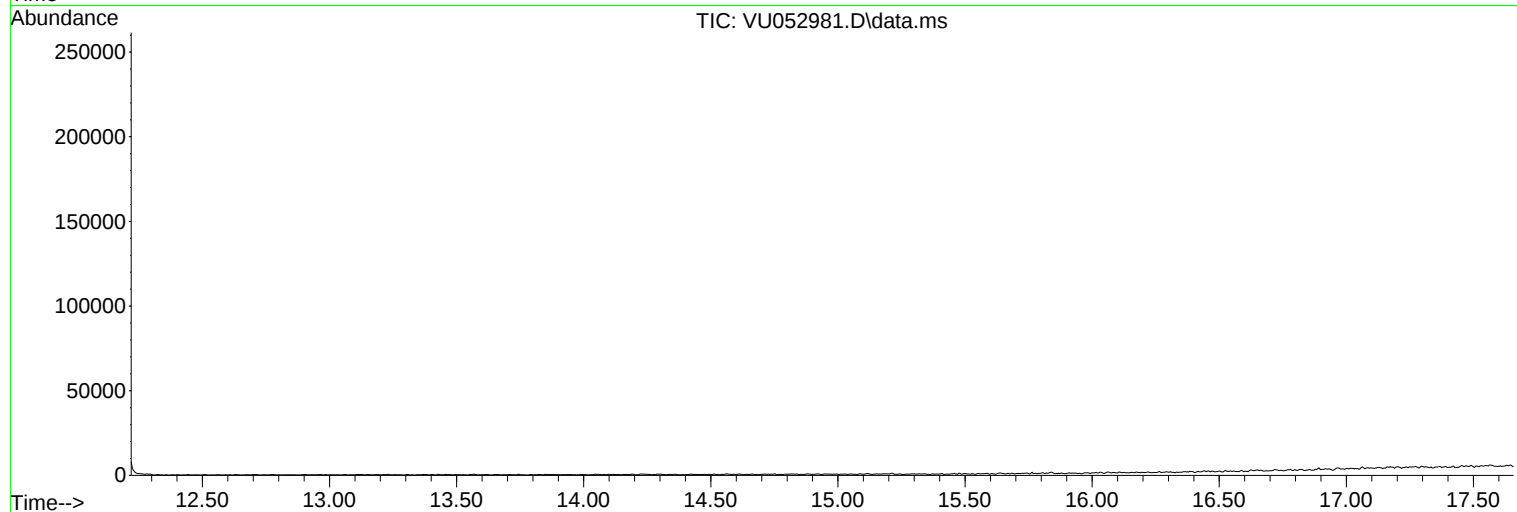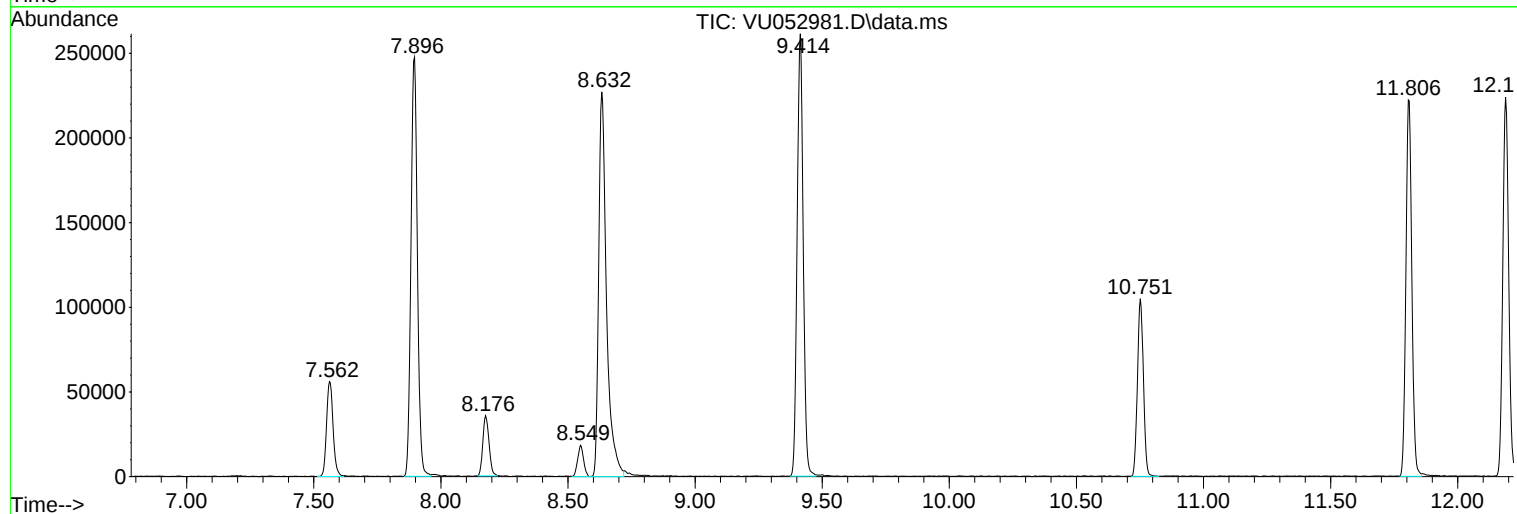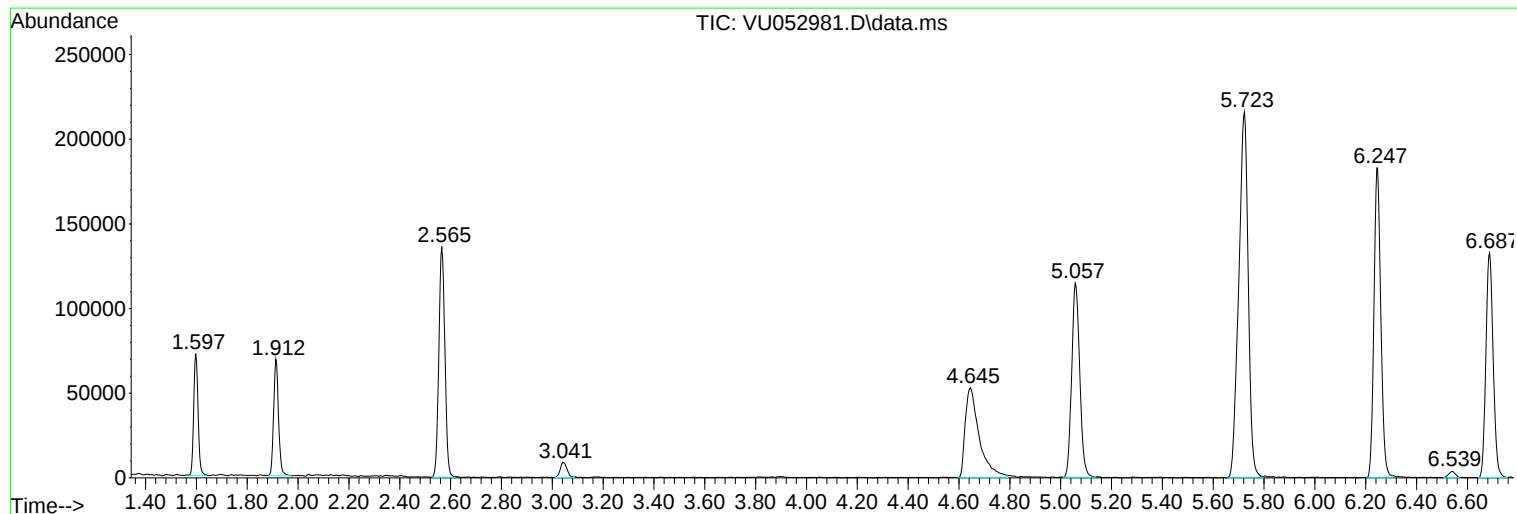

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052981.D
Acq On : 06 Feb 2023 15:29
Operator : JC/MD
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052981.D
Acq On : 06 Feb 2023 15:29
Operator : JC/MD
Sample : VIBLK145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
