

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052982.D
 Acq On : 06 Feb 2023 15:56
 Operator : JC/MD
 Sample : 01444-06 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	97	rVB	67318	84907	13.27%	1.466%
2	1.912	168	178	204	rVB	55687	89771	14.03%	1.551%
3	2.559	367	379	395	rVB2	151988	250782	39.21%	4.331%
4	3.041	517	529	548	rVB2	23450	45228	7.07%	0.781%
5	3.182	553	573	588	rBV	22315	55770	8.72%	0.963%
6	3.350	615	625	636	rVB4	6342	11699	1.83%	0.202%
7	4.658	1009	1032	1079	rBV4	112990	377554	59.03%	6.521%
8	5.057	1139	1156	1175	rBV2	118867	262569	41.05%	4.535%
9	5.719	1342	1362	1389	rBV2	237866	600965	93.96%	10.380%
10	6.243	1512	1525	1544	rBV	202889	387249	60.54%	6.688%
11	6.536	1601	1616	1640	rBV	338023	639625	100.00%	11.047%
12	6.687	1649	1663	1687	rVB	143910	278368	43.52%	4.808%
13	7.562	1924	1935	1950	rBV2	62122	110358	17.25%	1.906%
14	7.893	2025	2038	2057	rBV	275934	470728	73.59%	8.130%
15	8.176	2116	2126	2140	rBV	38664	64692	10.11%	1.117%
16	8.549	2230	2242	2256	rVB2	10749	16537	2.59%	0.286%
17	8.645	2256	2272	2309	rBV2	237332	544917	85.19%	9.412%
18	9.414	2493	2511	2531	rBV	285600	473667	74.05%	8.181%
19	10.754	2917	2928	2944	rBV	113596	184100	28.78%	3.180%
20	11.809	3241	3256	3281	rBV	268678	427860	66.89%	7.390%
21	12.192	3361	3375	3394	rBV	255125	412449	64.48%	7.124%




Sum of corrected areas: 5789795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052982.D
Acq On : 06 Feb 2023 15:56
Operator : JC/MD
Sample : 01444-06 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

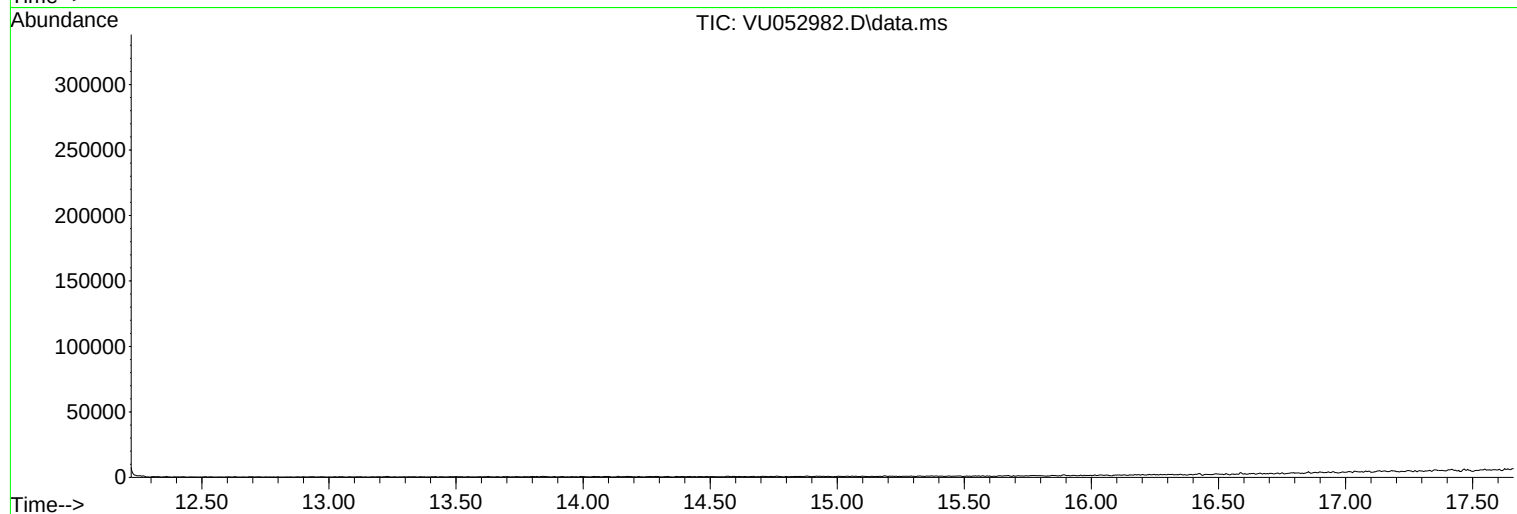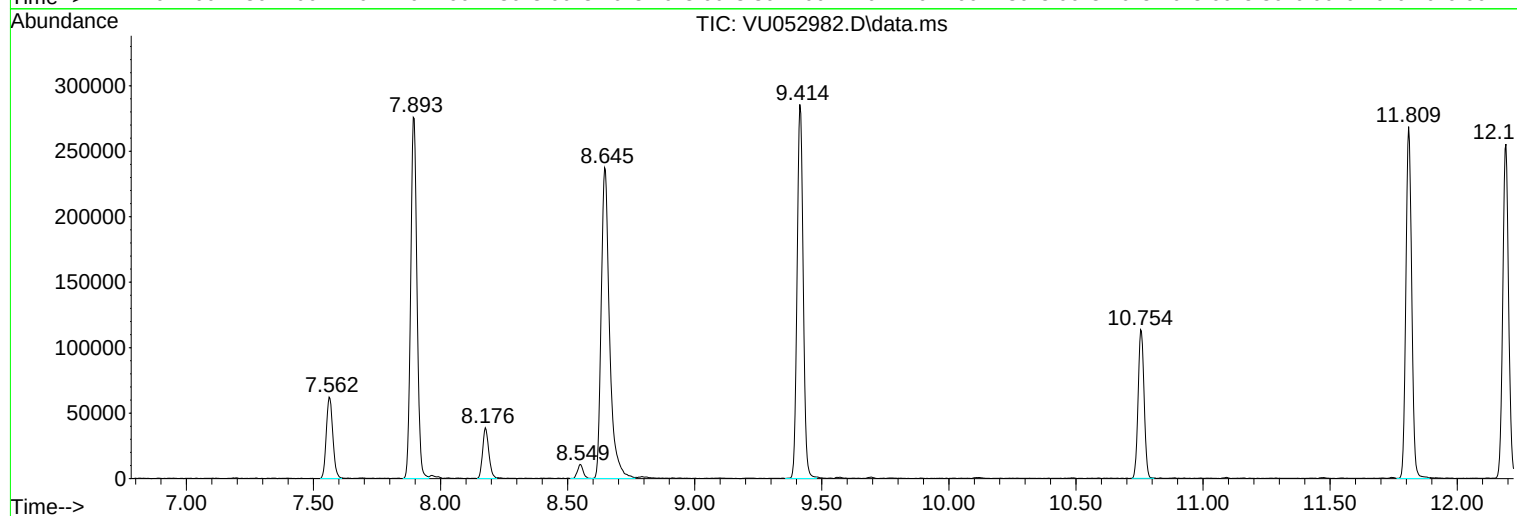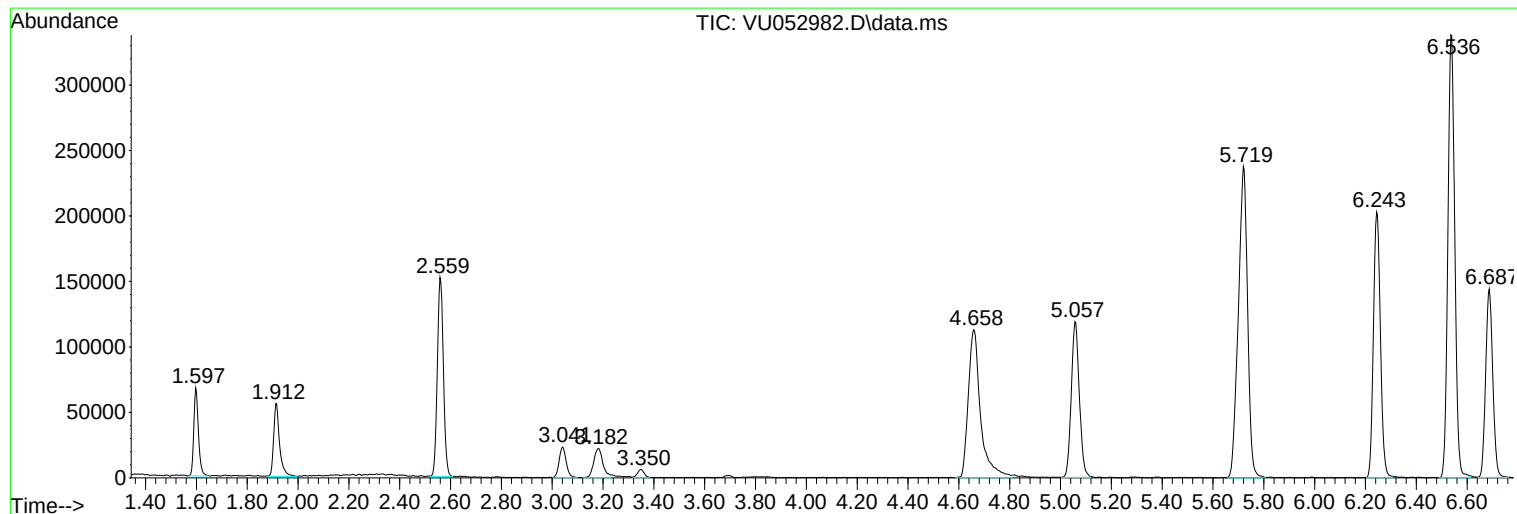

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052982.D
Acq On : 06 Feb 2023 15:56
Operator : JC/MD
Sample : 01444-06 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052982.D
Acq On : 06 Feb 2023 15:56
Operator : JC/MD
Sample : 01444-06 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc