

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052984.D
 Acq On : 06 Feb 2023 17:06
 Operator : JC/MD
 Sample : VIBLK146
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK146

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	93	rBV	49187	56254	10.47%	1.340%
2	1.912	169	178	194	rVB2	52037	68055	12.66%	1.621%
3	2.565	368	381	397	rBV	101979	166497	30.98%	3.965%
4	3.044	517	530	547	rVB2	20631	37862	7.05%	0.902%
5	4.645	1014	1028	1062	rBV2	60822	234499	43.64%	5.584%
6	5.057	1140	1156	1179	rVB	104369	228945	42.61%	5.452%
7	5.722	1340	1363	1389	rBV2	193962	501525	93.33%	11.943%
8	6.247	1513	1526	1544	rBV	165565	315389	58.69%	7.510%
9	6.687	1650	1663	1682	rBV	124314	243107	45.24%	5.789%
10	7.562	1923	1935	1951	rBV2	53448	91642	17.05%	2.182%
11	7.896	2025	2039	2056	rBV	215724	373091	69.43%	8.884%
12	8.176	2116	2126	2143	rBV2	32409	55374	10.30%	1.319%
13	8.549	2233	2242	2250	rBV5	3910	6178	1.15%	0.147%
14	8.632	2254	2268	2298	rBV3	251763	537355	100.00%	12.796%
15	9.414	2495	2511	2534	rBV	240866	399132	74.28%	9.505%
16	10.751	2911	2927	2946	rBV	108129	172438	32.09%	4.106%
17	11.806	3244	3255	3272	rBV	213202	344197	64.05%	8.196%
18	12.188	3360	3374	3399	rBV	207498	340343	63.34%	8.105%
19	13.841	3879	3888	3899	rVB3	6100	9320	1.73%	0.222%
20	14.089	3956	3965	3977	rBV2	5047	8367	1.56%	0.199%
21	14.327	4028	4039	4049	rBV5	5809	9778	1.82%	0.233%




Sum of corrected areas: 4199348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052984.D
Acq On : 06 Feb 2023 17:06
Operator : JC/MD
Sample : VIBLK146
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

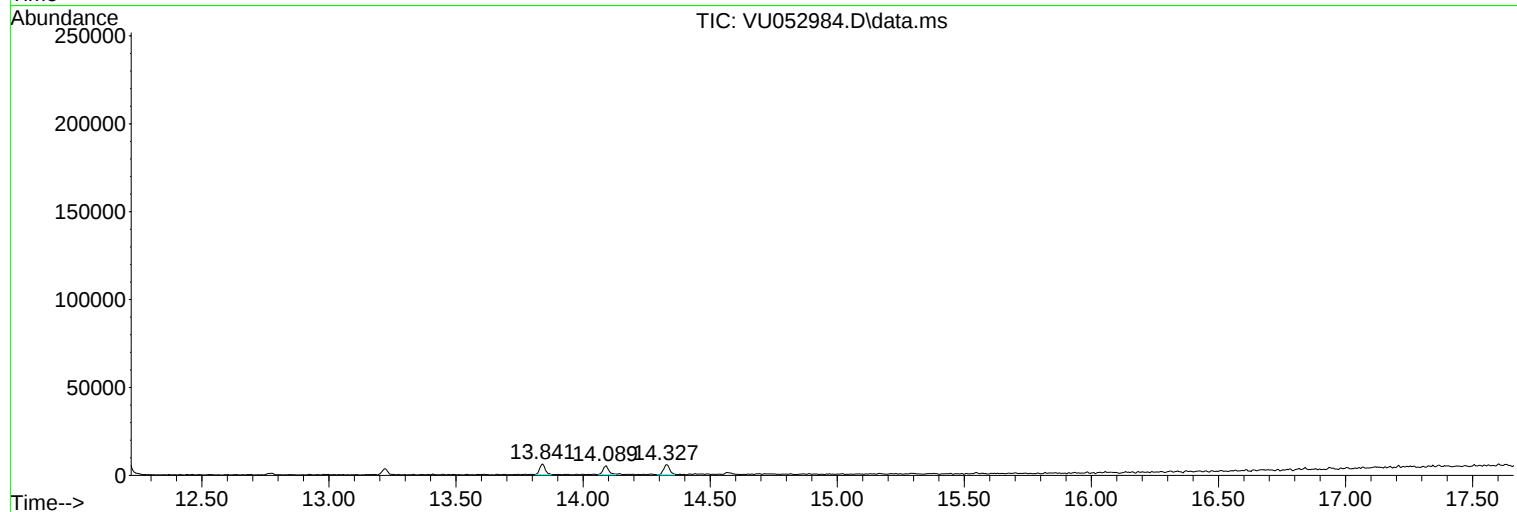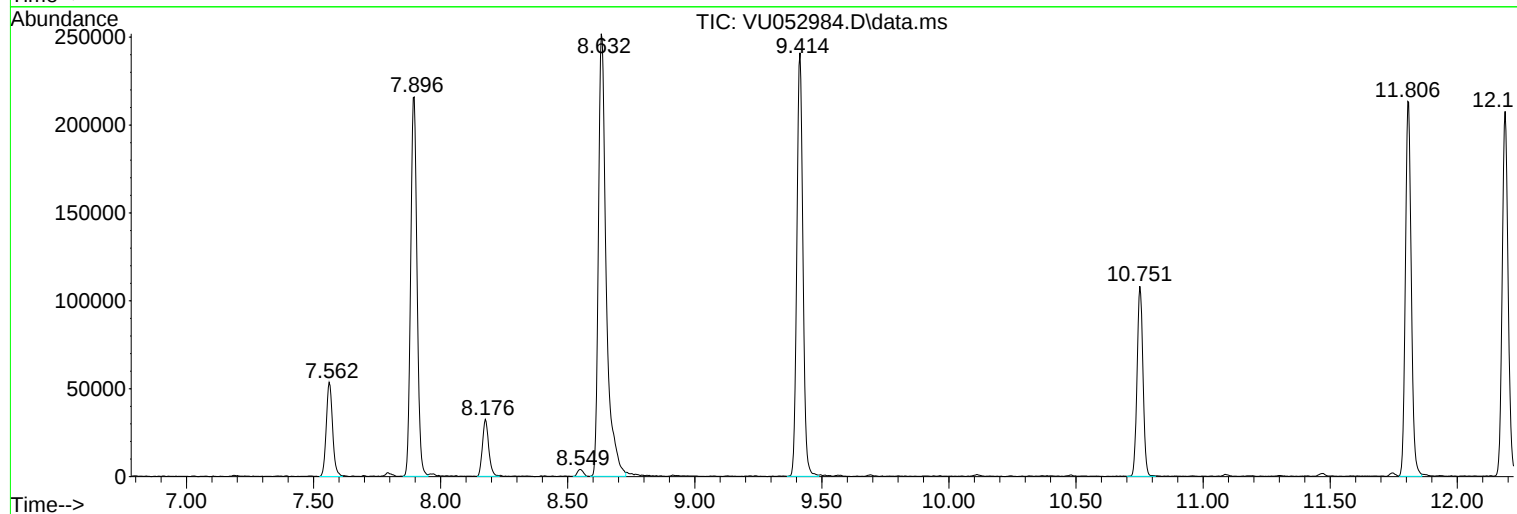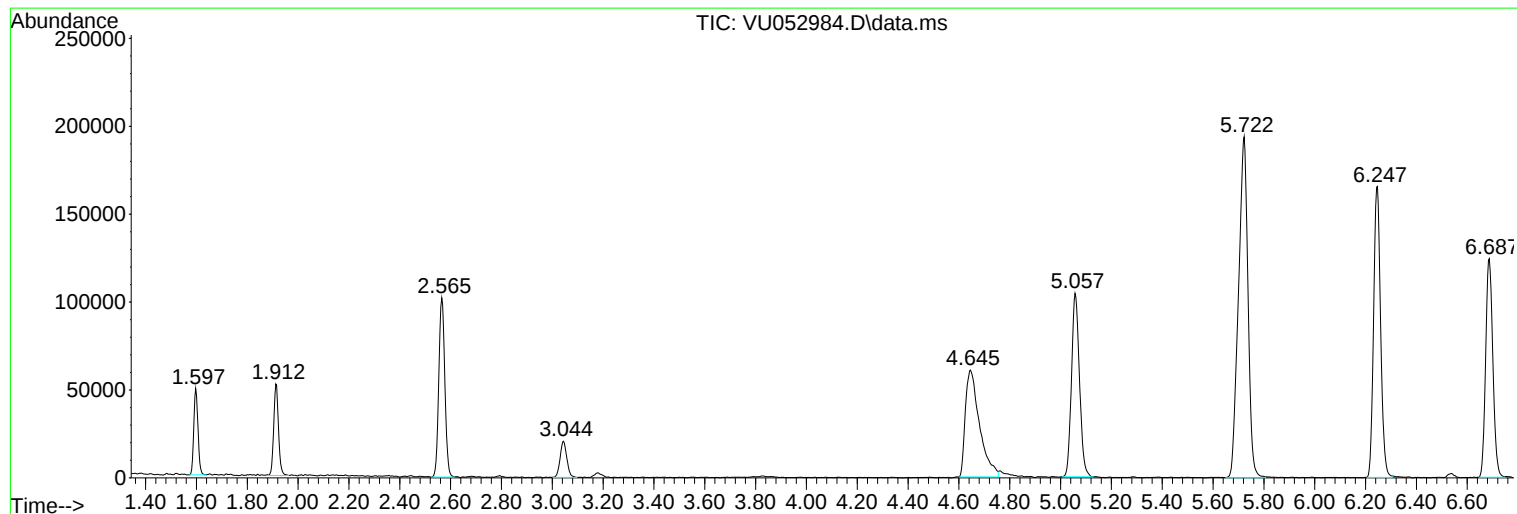

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052984.D
Acq On : 06 Feb 2023 17:06
Operator : JC/MD
Sample : VIBLK146
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052984.D
Acq On : 06 Feb 2023 17:06
Operator : JC/MD
Sample : VIBLK146
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc