

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052986.D
 Acq On : 06 Feb 2023 17:55
 Operator : JC/MD
 Sample : 01444-08 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	93	rBV	67702	81262	9.30%	1.466%
2	1.912	168	178	195	rBV	62376	82375	9.42%	1.487%
3	2.565	369	381	398	rVB2	137468	227689	26.05%	4.109%
4	3.044	520	530	548	rVB2	8824	15983	1.83%	0.288%
5	3.179	558	572	588	rBV	6899	15300	1.75%	0.276%
6	3.353	615	626	640	rVB3	7391	14010	1.60%	0.253%
7	4.658	1009	1032	1057	rBV4	120118	405213	46.35%	7.312%
8	5.057	1139	1156	1178	rBV	110458	247659	28.33%	4.469%
9	5.723	1341	1363	1385	rBV2	210995	550665	62.99%	9.937%
10	6.243	1512	1525	1548	rBV	185174	355462	40.66%	6.415%
11	6.539	1601	1617	1641	rBV	461470	874172	100.00%	15.775%
12	6.687	1649	1663	1681	rVB	133512	258159	29.53%	4.659%
13	7.562	1924	1935	1956	rBV2	55024	99124	11.34%	1.789%
14	7.893	2026	2038	2055	rBV	251291	433590	49.60%	7.824%
15	8.176	2116	2126	2143	rBV2	34725	58784	6.72%	1.061%
16	8.632	2256	2268	2301	rBV3	223916	478541	54.74%	8.636%
17	9.414	2498	2511	2533	rBV	270170	444302	50.83%	8.018%
18	10.751	2915	2927	2947	rBV2	100523	163761	18.73%	2.955%
19	11.806	3244	3255	3275	rBV	236421	377064	43.13%	6.804%
20	12.189	3361	3374	3400	rBV	215462	358353	40.99%	6.467%




Sum of corrected areas: 5541468

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052986.D
Acq On : 06 Feb 2023 17:55
Operator : JC/MD
Sample : 01444-08 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

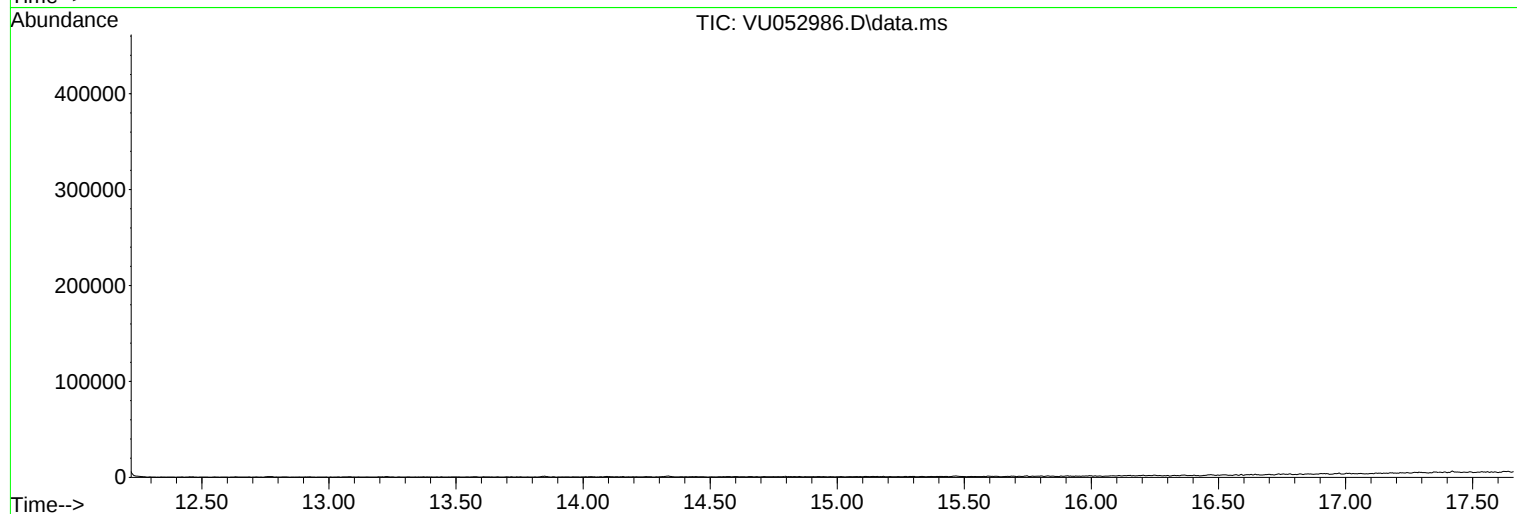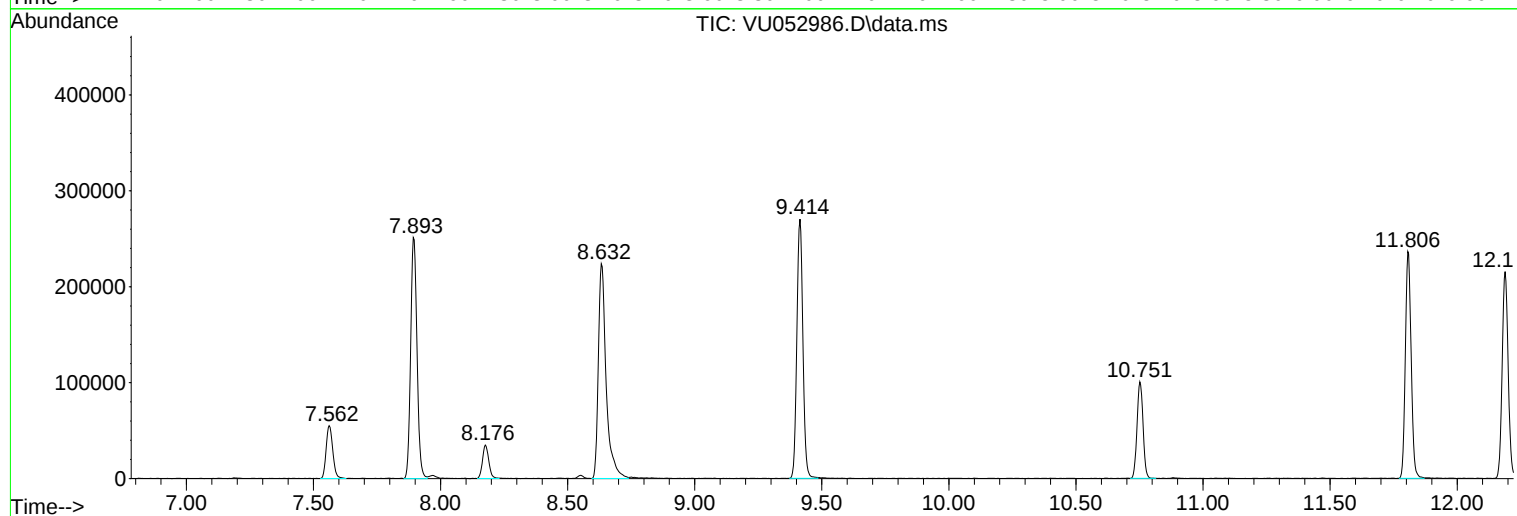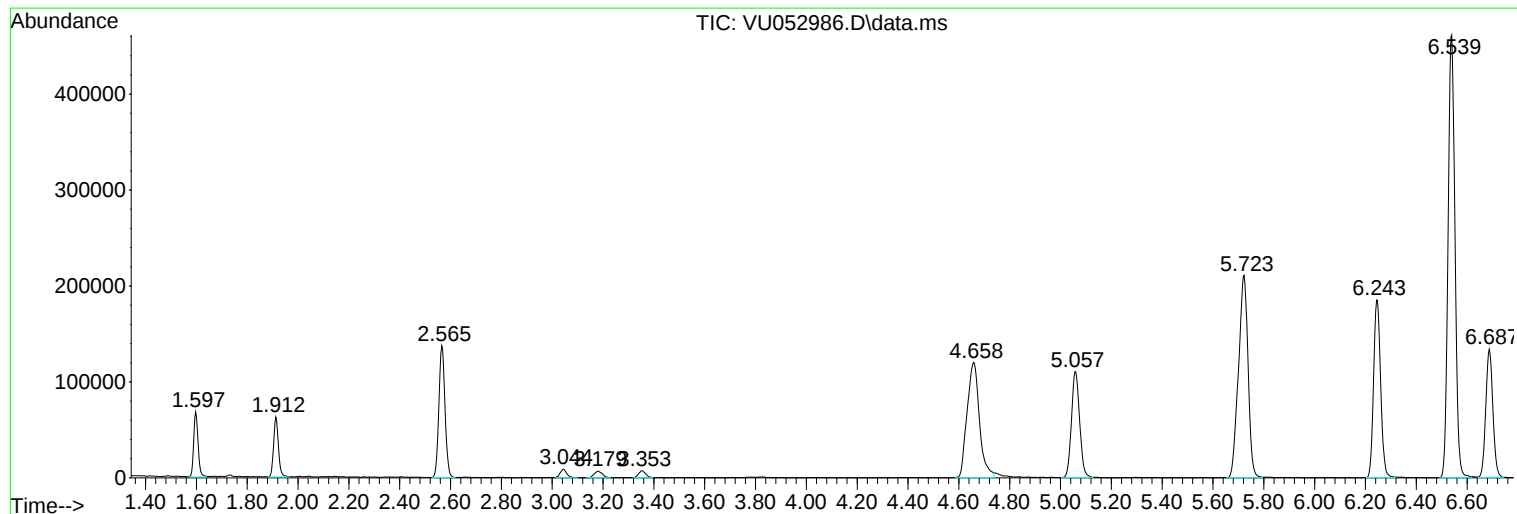

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052986.D
Acq On : 06 Feb 2023 17:55
Operator : JC/MD
Sample : 01444-08 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052986.D
Acq On : 06 Feb 2023 17:55
Operator : JC/MD
Sample : 01444-08 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc