

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052988.D
 Acq On : 06 Feb 2023 18:43
 Operator : JC/MD
 Sample : 01444-10 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	70	80	94	rBV	44900	56280	7.70%	1.057%
2	1.912	169	178	200	rVB	41975	65140	8.91%	1.224%
3	2.559	366	379	394	rVB2	110851	185461	25.37%	3.484%
4	3.041	514	529	554	rVB2	22487	45293	6.19%	0.851%
5	3.179	554	572	595	rBV2	30511	76047	10.40%	1.428%
6	4.655	1010	1031	1074	rBV4	94171	343951	47.04%	6.461%
7	5.057	1137	1156	1179	rBV	106256	235565	32.22%	4.425%
8	5.719	1342	1362	1385	rBV2	199233	519170	71.01%	9.752%
9	6.243	1509	1525	1545	rBV	175253	333618	45.63%	6.266%
10	6.536	1602	1616	1633	rBV	385363	731151	100.00%	13.733%
11	6.684	1647	1662	1681	rBV	128250	251568	34.41%	4.725%
12	7.562	1924	1935	1949	rBV2	54391	95043	13.00%	1.785%
13	7.893	2023	2038	2055	rBV	221576	388836	53.18%	7.304%
14	8.176	2116	2126	2143	rBV2	34079	58190	7.96%	1.093%
15	8.645	2258	2272	2310	rBV3	254252	586635	80.23%	11.019%
16	9.414	2497	2511	2530	rBV	246464	413366	56.54%	7.764%
17	10.755	2916	2928	2941	rBV	116640	186457	25.50%	3.502%
18	11.809	3244	3256	3270	rBV	238541	381450	52.17%	7.165%
19	12.192	3361	3375	3392	rBV	229645	370676	50.70%	6.962%




Sum of corrected areas: 5323897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052988.D
Acq On : 06 Feb 2023 18:43
Operator : JC/MD
Sample : 01444-10 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

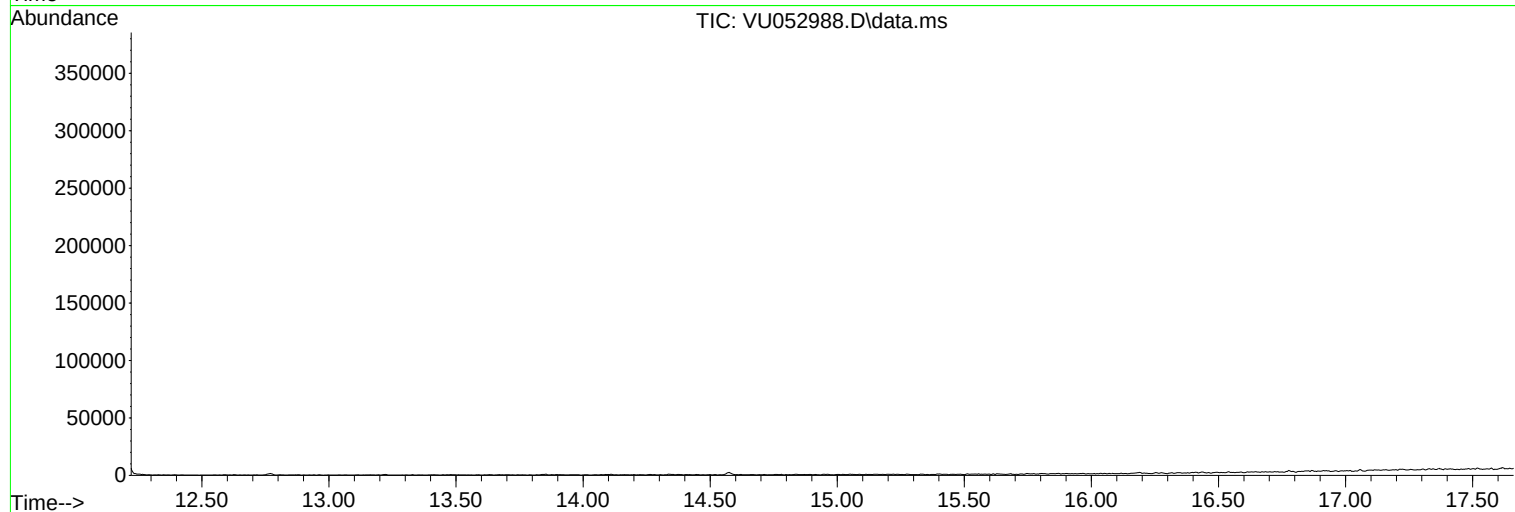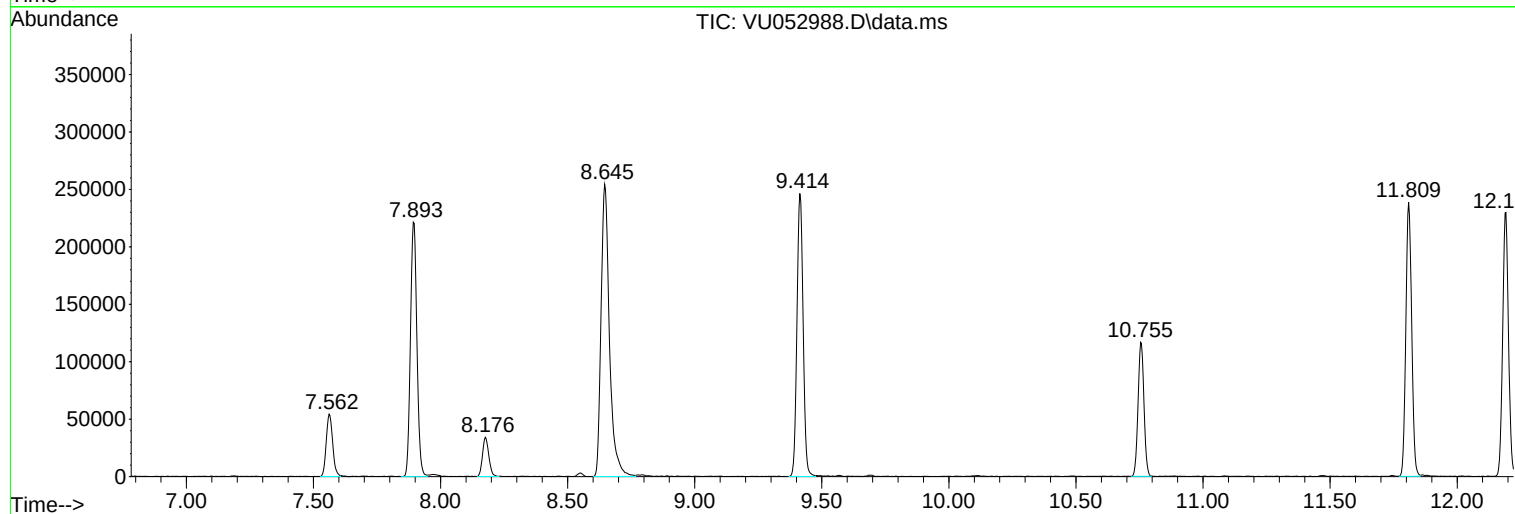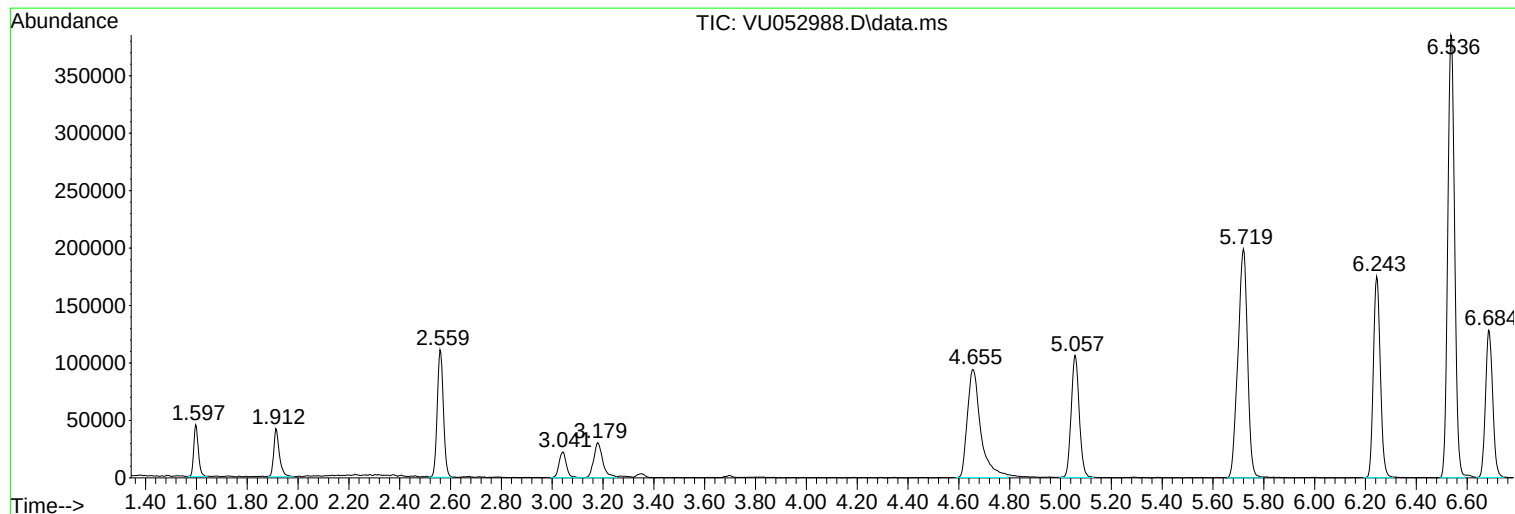

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052988.D
Acq On : 06 Feb 2023 18:43
Operator : JC/MD
Sample : 01444-10 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052988.D
Acq On : 06 Feb 2023 18:43
Operator : JC/MD
Sample : 01444-10 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc