

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052989.D
 Acq On : 06 Feb 2023 19:07
 Operator : JC/MD
 Sample : 01444-11 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM15

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	69	80	92	rBV	45971	52697	6.33%	1.080%
2	1.912	169	178	190	rBV	45190	61123	7.34%	1.252%
3	2.565	370	381	395	rBV2	93711	158604	19.04%	3.249%
4	3.044	518	530	543	rBV2	7613	14143	1.70%	0.290%
5	3.179	557	572	588	rBV2	5969	13770	1.65%	0.282%
6	4.652	1007	1030	1072	rBV4	88745	344651	41.38%	7.060%
7	5.060	1140	1157	1178	rBV	101424	223442	26.83%	4.577%
8	5.723	1338	1363	1392	rBV2	178959	469735	56.40%	9.623%
9	6.243	1513	1525	1547	rBV	162145	307995	36.98%	6.309%
10	6.539	1601	1617	1635	rBV	446912	832923	100.00%	17.063%
11	6.687	1650	1663	1681	rVB	117825	230701	27.70%	4.726%
12	7.562	1924	1935	1952	rBV	48290	85134	10.22%	1.744%
13	7.893	2025	2038	2059	rBV	196005	342058	41.07%	7.007%
14	8.176	2116	2126	2142	rBV	29952	50742	6.09%	1.039%
15	8.632	2255	2268	2301	rBV3	243409	505468	60.69%	10.355%
16	9.414	2498	2511	2528	rBV	230672	385052	46.23%	7.888%
17	10.751	2915	2927	2945	rBV	103760	165354	19.85%	3.387%
18	11.806	3243	3255	3277	rBV	203359	327235	39.29%	6.704%
19	12.189	3363	3374	3391	rBV	190855	310668	37.30%	6.364%




Sum of corrected areas: 4881495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052989.D
Acq On : 06 Feb 2023 19:07
Operator : JC/MD
Sample : 01444-11 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

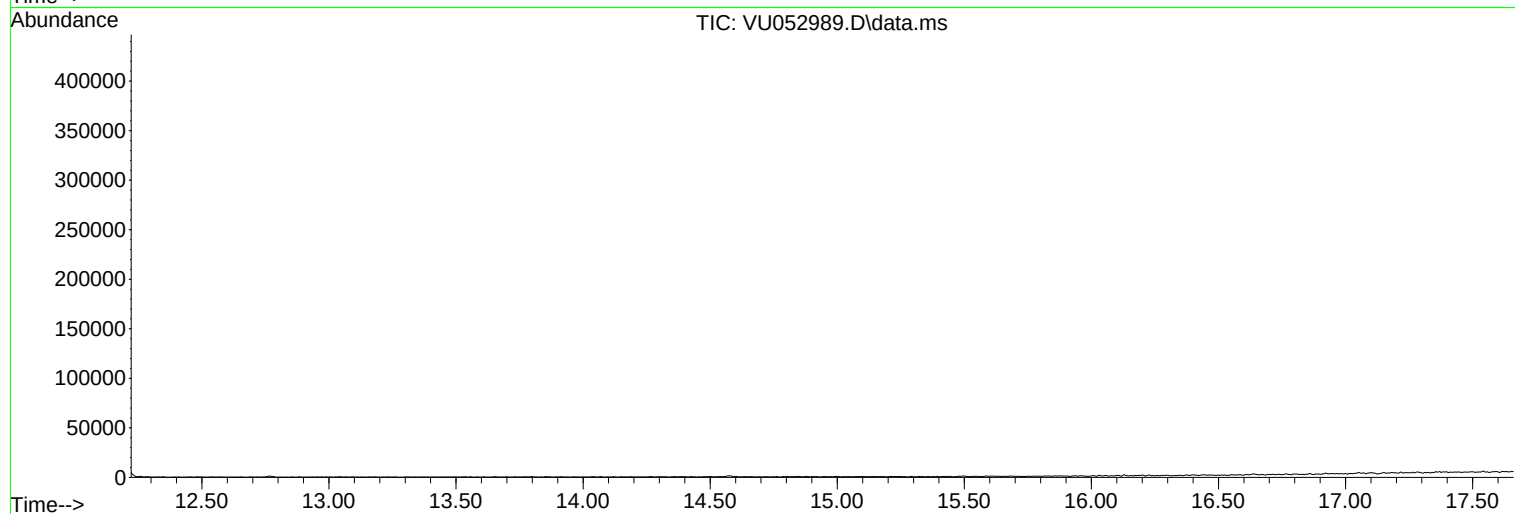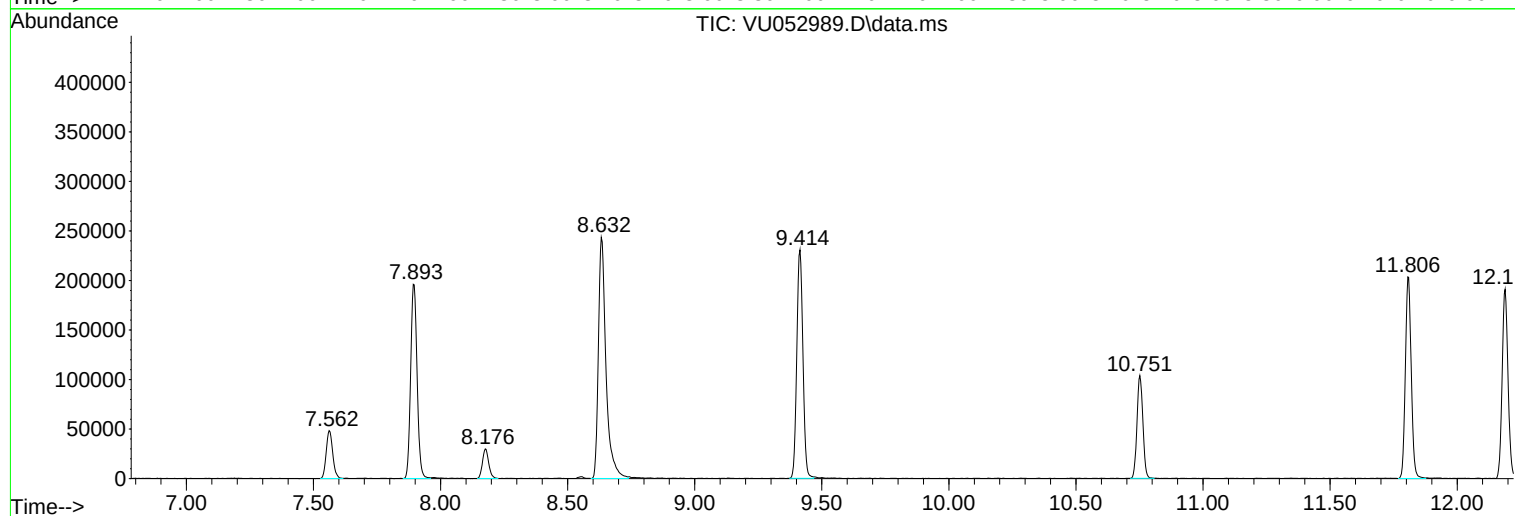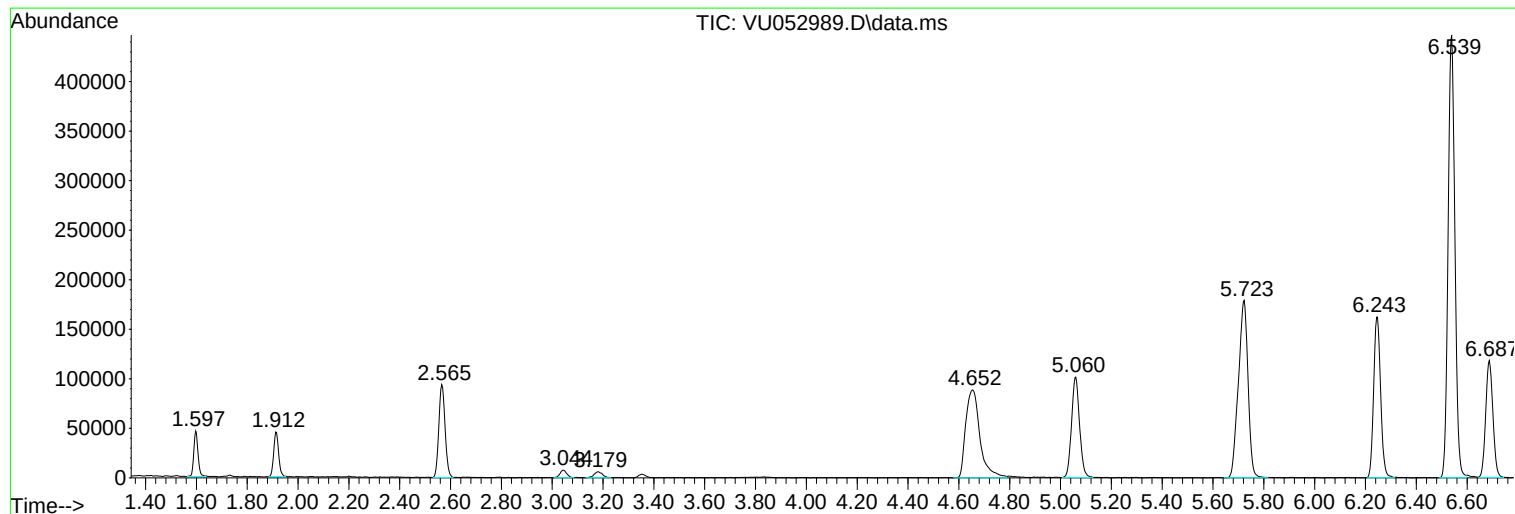

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052989.D
Acq On : 06 Feb 2023 19:07
Operator : JC/MD
Sample : 01444-11 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052989.D
Acq On : 06 Feb 2023 19:07
Operator : JC/MD
Sample : 01444-11 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------