

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052990.D
 Acq On : 06 Feb 2023 19:31
 Operator : JC/MD
 Sample : 01444-12 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM16

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rVB	44642	52814	7.19%	1.097%
2	1.912	168	178	194	rVB	48307	63017	8.58%	1.309%
3	2.565	369	381	397	rVB2	95558	161084	21.92%	3.347%
4	3.044	520	530	544	rVB2	7794	15060	2.05%	0.313%
5	3.182	559	573	586	rBV2	9745	22716	3.09%	0.472%
6	4.652	1008	1030	1065	rBV3	80053	308161	41.94%	6.403%
7	5.057	1136	1156	1176	rBV	98873	220504	30.01%	4.581%
8	5.722	1342	1363	1387	rBV2	176787	466687	63.51%	9.696%
9	6.247	1512	1526	1544	rBV	167048	314074	42.74%	6.525%
10	6.539	1603	1617	1634	rBV	390140	734787	100.00%	15.267%
11	6.687	1649	1663	1681	rBV	118644	231389	31.49%	4.808%
12	7.562	1924	1935	1950	rBV	48486	84910	11.56%	1.764%
13	7.896	2024	2039	2055	rBV	199513	344698	46.91%	7.162%
14	8.176	2115	2126	2146	rVB2	31072	51785	7.05%	1.076%
15	8.632	2256	2268	2300	rBV3	242232	504973	68.72%	10.492%
16	9.414	2499	2511	2537	rBV	243209	401384	54.63%	8.339%
17	10.751	2915	2927	2942	rBV	103103	165105	22.47%	3.430%
18	11.806	3244	3255	3275	rBV	217828	347733	47.32%	7.225%
19	12.188	3362	3374	3390	rBV	196654	322168	43.85%	6.694%




Sum of corrected areas: 4813049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052990.D
Acq On : 06 Feb 2023 19:31
Operator : JC/MD
Sample : 01444-12 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

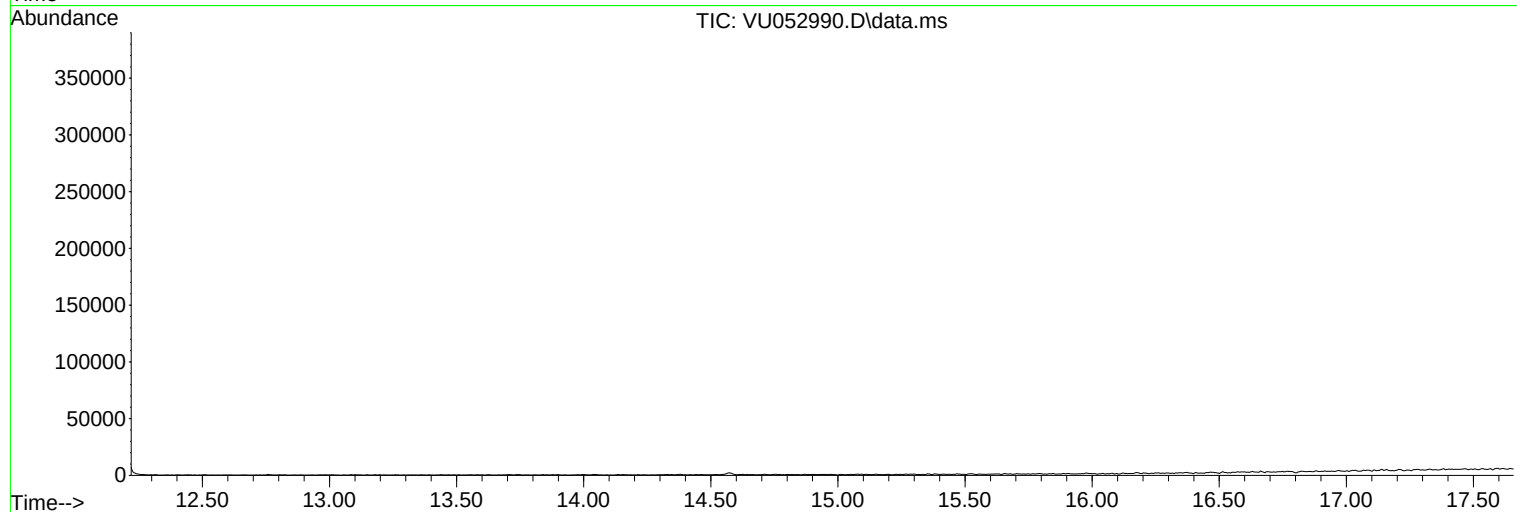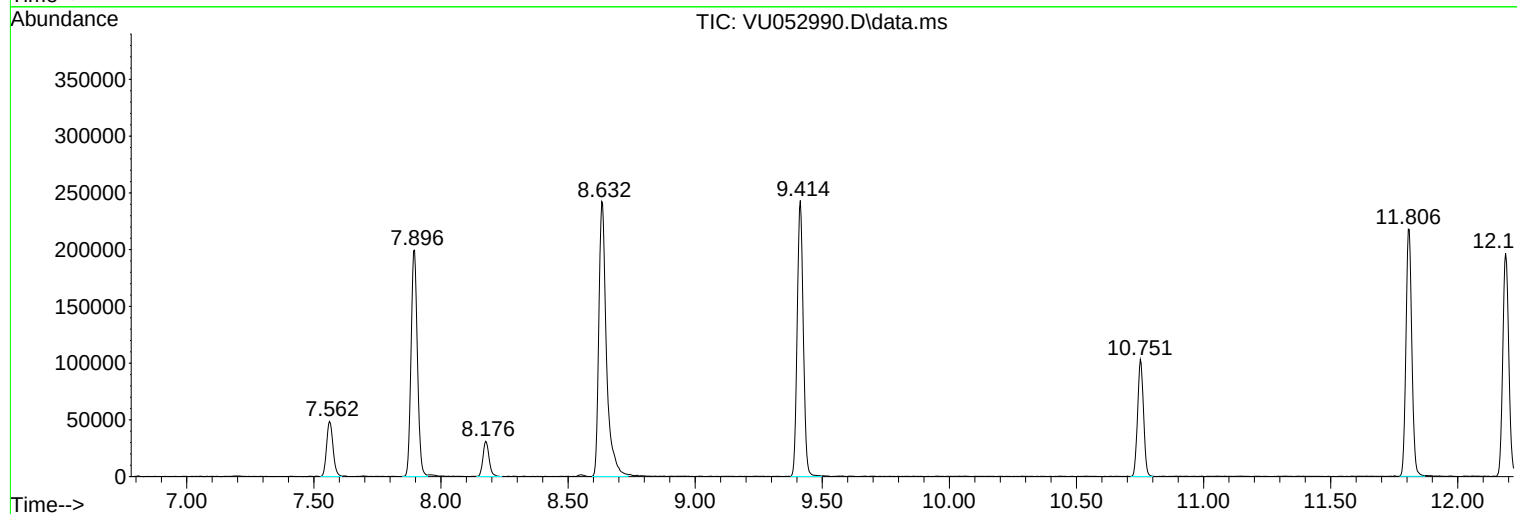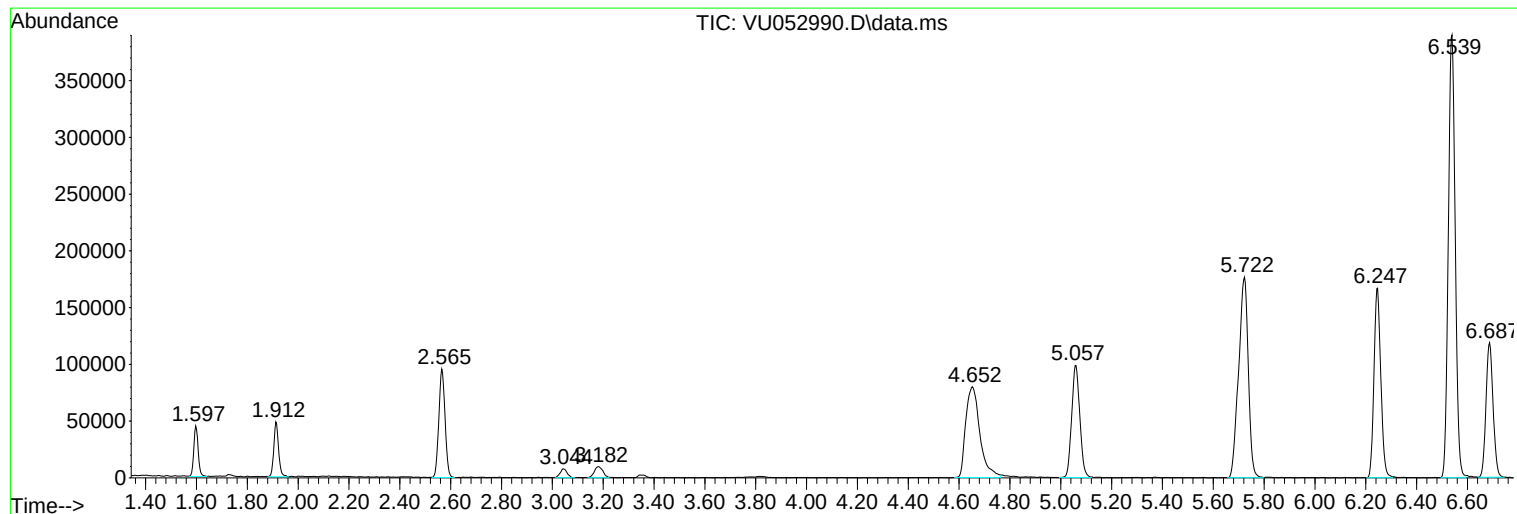

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052990.D
Acq On : 06 Feb 2023 19:31
Operator : JC/MD
Sample : 01444-12 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052990.D
Acq On : 06 Feb 2023 19:31
Operator : JC/MD
Sample : 01444-12 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc