

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052991.D
 Acq On : 06 Feb 2023 19:56
 Operator : JC/MD
 Sample : 01444-05 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	92	rBV	49384	57336	5.01%	1.022%
2	1.912	169	178	193	rBV	49940	66191	5.78%	1.179%
3	2.565	369	381	396	rVB2	105114	180051	15.73%	3.208%
4	3.044	517	530	551	rVB3	19678	37490	3.28%	0.668%
5	3.353	614	626	642	rVB2	9754	19303	1.69%	0.344%
6	4.658	1012	1032	1071	rBV2	159445	505587	44.18%	9.008%
7	5.057	1140	1156	1179	rBV	108673	242419	21.18%	4.319%
8	5.723	1338	1363	1383	rBV2	191622	507136	44.31%	9.036%
9	6.243	1511	1525	1544	rBV	154394	298862	26.11%	5.325%
10	6.539	1603	1617	1634	rBV	611928	1144457	100.00%	20.392%
11	6.687	1649	1663	1684	rVB	128858	253397	22.14%	4.515%
12	7.562	1917	1935	1951	rBV	55069	95777	8.37%	1.707%
13	7.896	2026	2039	2056	rBV	211120	372560	32.55%	6.638%
14	8.176	2116	2126	2145	rBV	33346	55754	4.87%	0.993%
15	8.632	2256	2268	2300	rBV3	266680	561172	49.03%	9.999%
16	9.414	2499	2511	2534	rBV	224523	375017	32.77%	6.682%
17	10.751	2914	2927	2943	rBV	113065	181839	15.89%	3.240%
18	11.806	3242	3255	3275	rBV	199839	317443	27.74%	5.656%
19	12.188	3361	3374	3392	rBV	207486	340542	29.76%	6.068%




Sum of corrected areas: 5612333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052991.D
Acq On : 06 Feb 2023 19:56
Operator : JC/MD
Sample : 01444-05 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

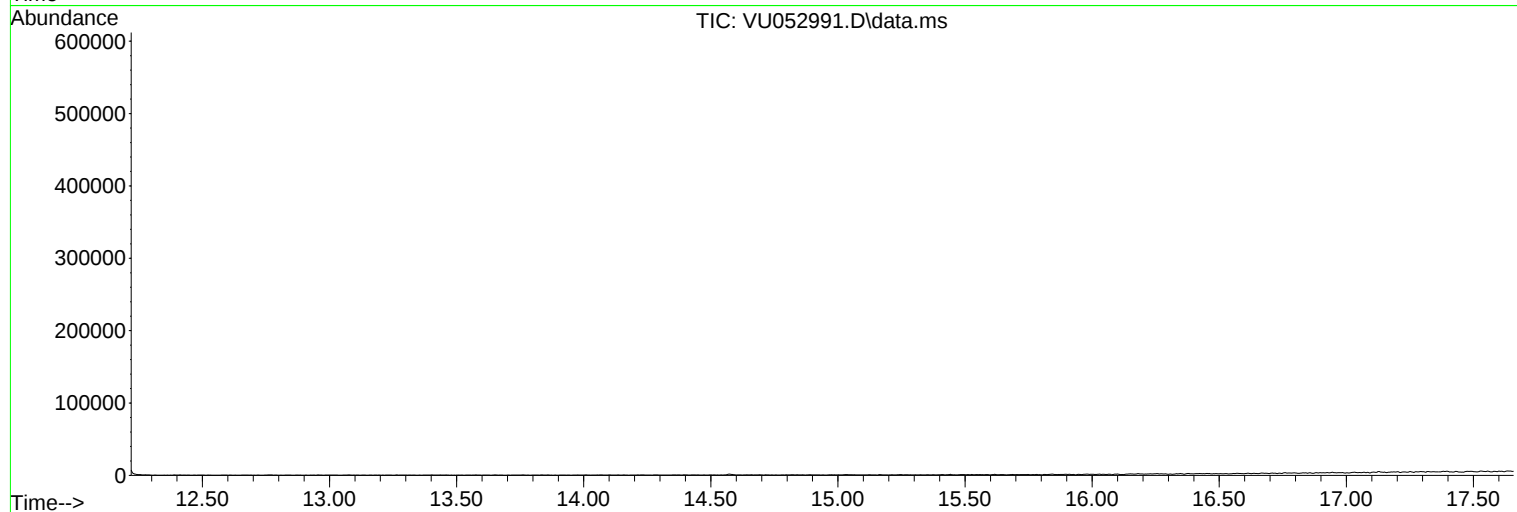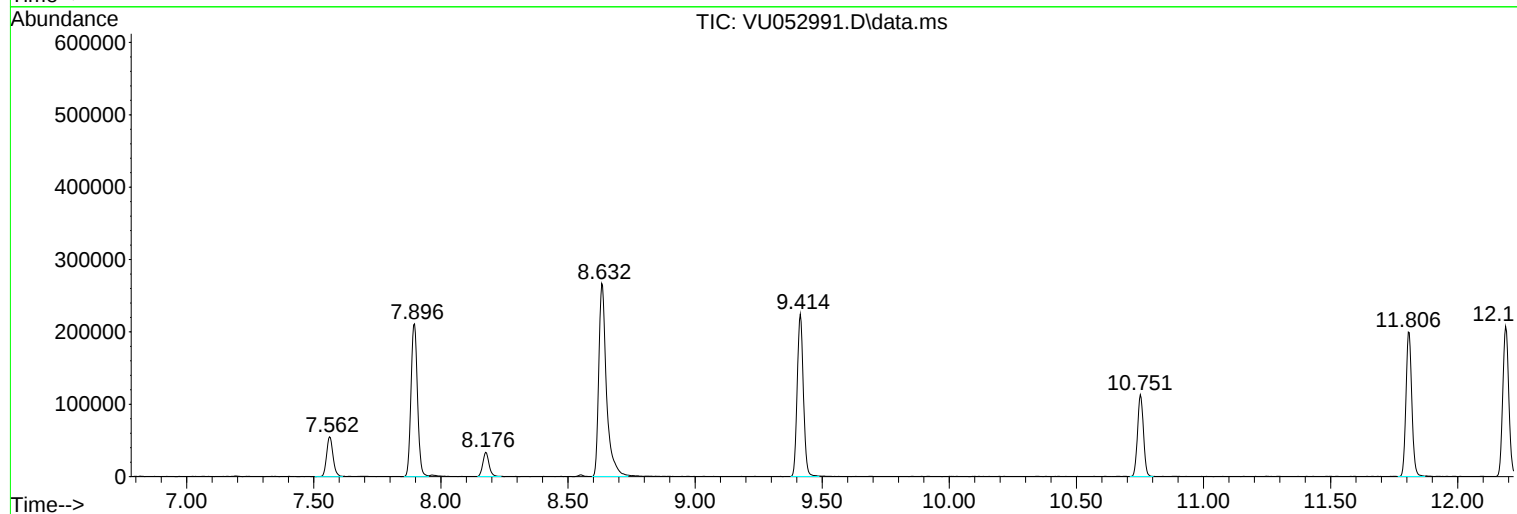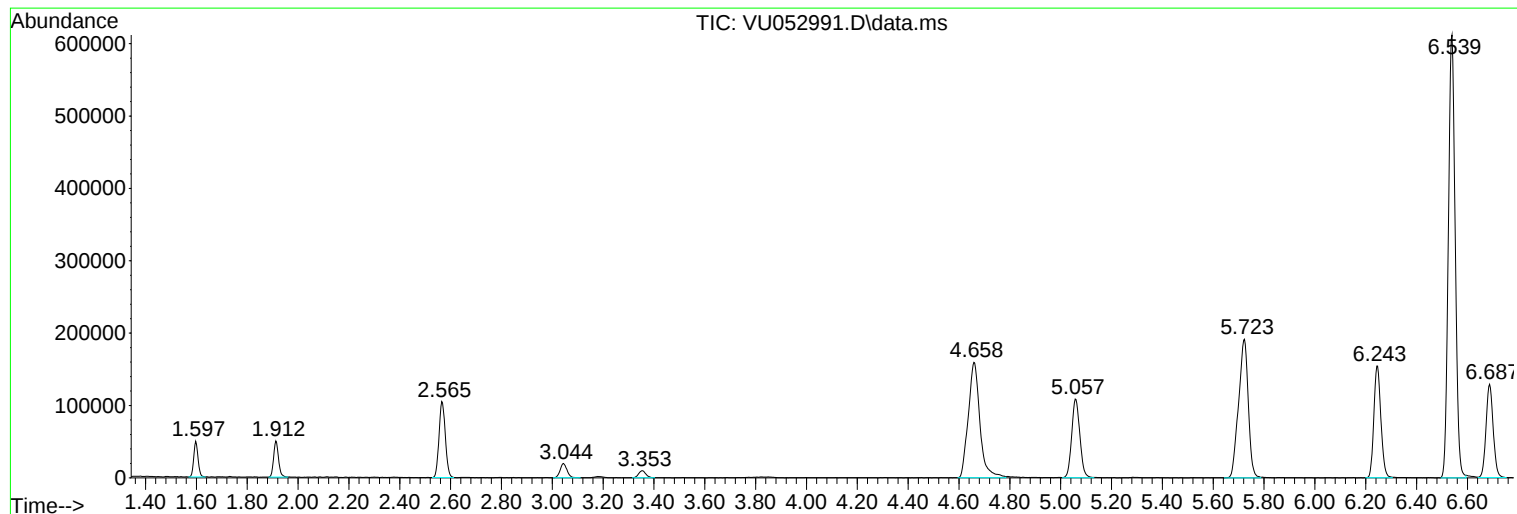

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052991.D
Acq On : 06 Feb 2023 19:56
Operator : JC/MD
Sample : 01444-05 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052991.D
Acq On : 06 Feb 2023 19:56
Operator : JC/MD
Sample : 01444-05 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc