

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
 Data File : VU052992.D
 Acq On : 06 Feb 2023 20:19
 Operator : JC/MD
 Sample : 01422-09DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B69DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	92	rBV2	52216	60157	11.01%	1.265%
2	1.913	169	178	190	rBV	47731	63092	11.55%	1.327%
3	2.565	366	381	396	rBV	95597	158438	29.00%	3.331%
4	3.044	514	530	548	rBV3	21783	40397	7.39%	0.849%
5	4.655	1013	1031	1067	rBV3	85409	316337	57.91%	6.651%
6	5.057	1136	1156	1179	rBV2	102861	233367	42.72%	4.907%
7	5.723	1343	1363	1385	rBV2	184647	489588	89.62%	10.294%
8	6.244	1512	1525	1549	rBV2	160518	307660	56.32%	6.469%
9	6.539	1602	1617	1634	rBV2	41987	79316	14.52%	1.668%
10	6.687	1650	1663	1680	rBV2	121941	239596	43.86%	5.037%
11	7.562	1924	1935	1950	rBV	51898	89816	16.44%	1.888%
12	7.893	2022	2038	2054	rBV	203176	353249	64.66%	7.427%
13	7.964	2054	2060	2076	rVB	5242	10175	1.86%	0.214%
14	8.176	2115	2126	2140	rBV	31557	53490	9.79%	1.125%
15	8.549	2229	2242	2256	rBV	289387	486882	89.13%	10.237%
16	8.632	2256	2268	2305	rVB2	256993	546278	100.00%	11.485%
17	9.414	2497	2511	2531	rBV	232887	391696	71.70%	8.235%
18	10.751	2915	2927	2944	rVB	108378	173763	31.81%	3.653%
19	11.806	3243	3255	3272	rBV2	206640	332589	60.88%	6.993%
20	12.189	3361	3374	3397	rBV	202320	330371	60.48%	6.946%




Sum of corrected areas: 4756257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052992.D
Acq On : 06 Feb 2023 20:19
Operator : JC/MD
Sample : 01422-09DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

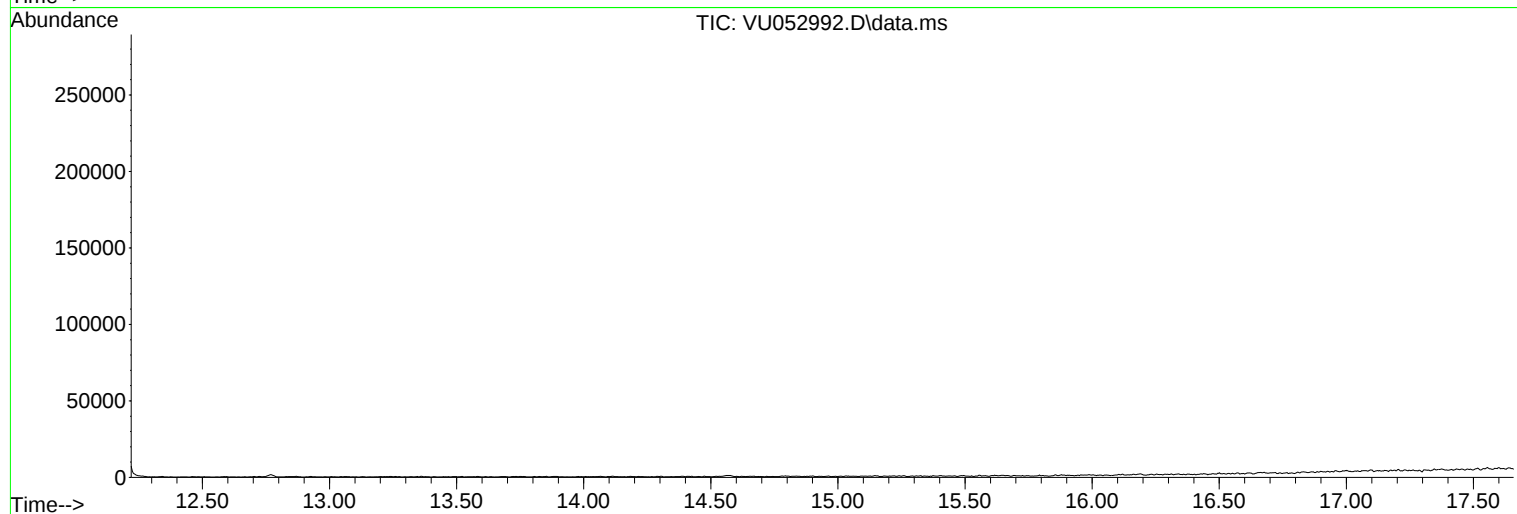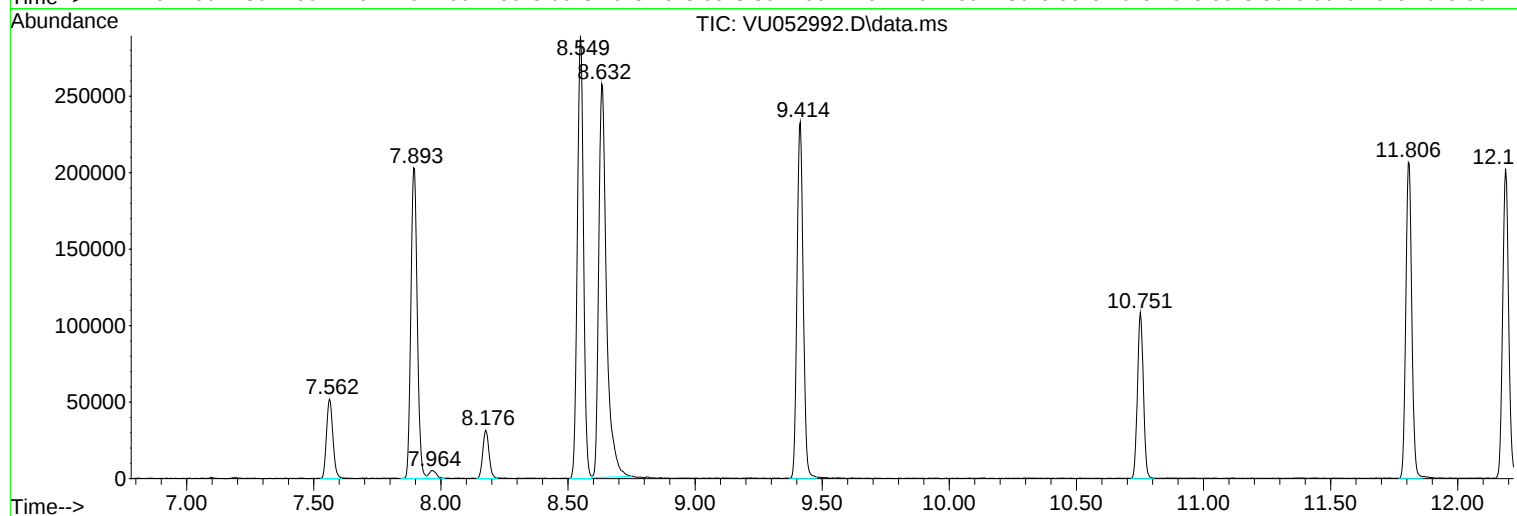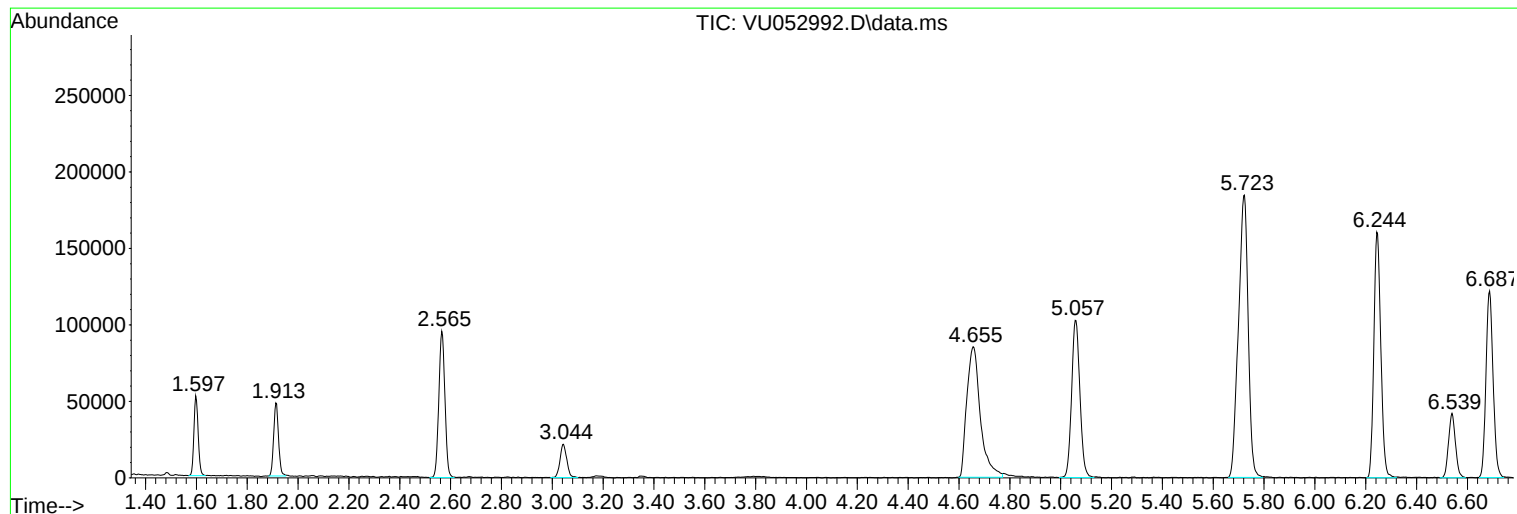

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052992.D
Acq On : 06 Feb 2023 20:19
Operator : JC/MD
Sample : 01422-09DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052992.D
Acq On : 06 Feb 2023 20:19
Operator : JC/MD
Sample : 01422-09DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc