
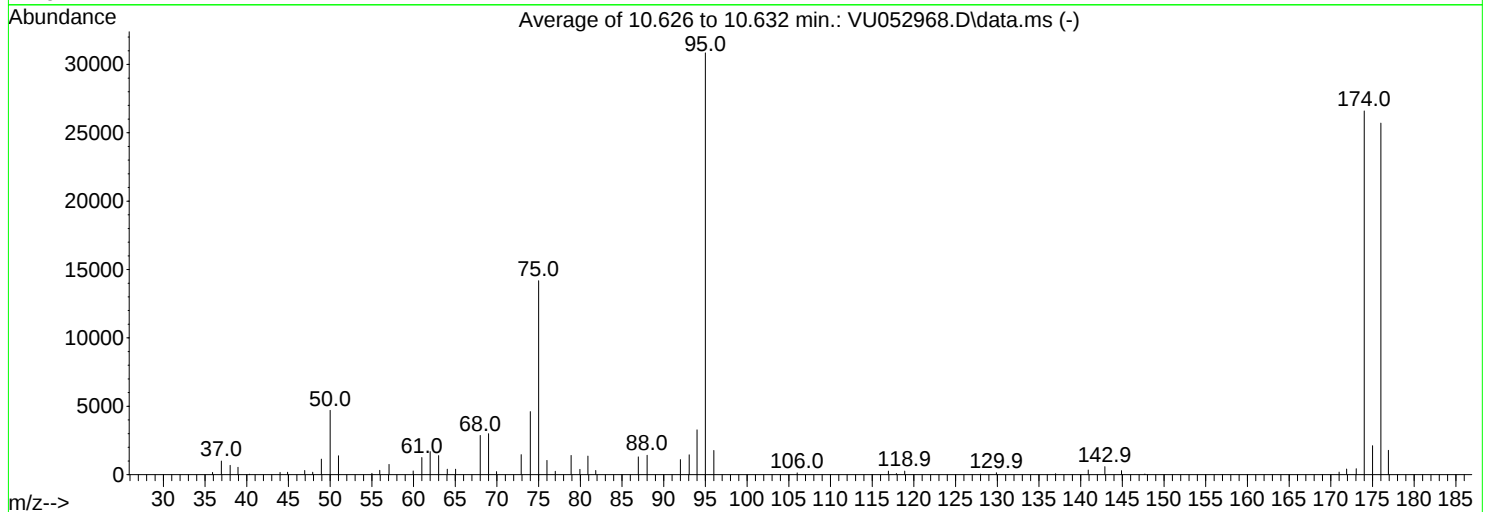


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020623\
Data File : VU052968.D
Acq On : 06 Feb 2023 08:54
Operator : JC/MD
Sample : BFB194
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB194

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sun Feb 05 21:58:05 2023

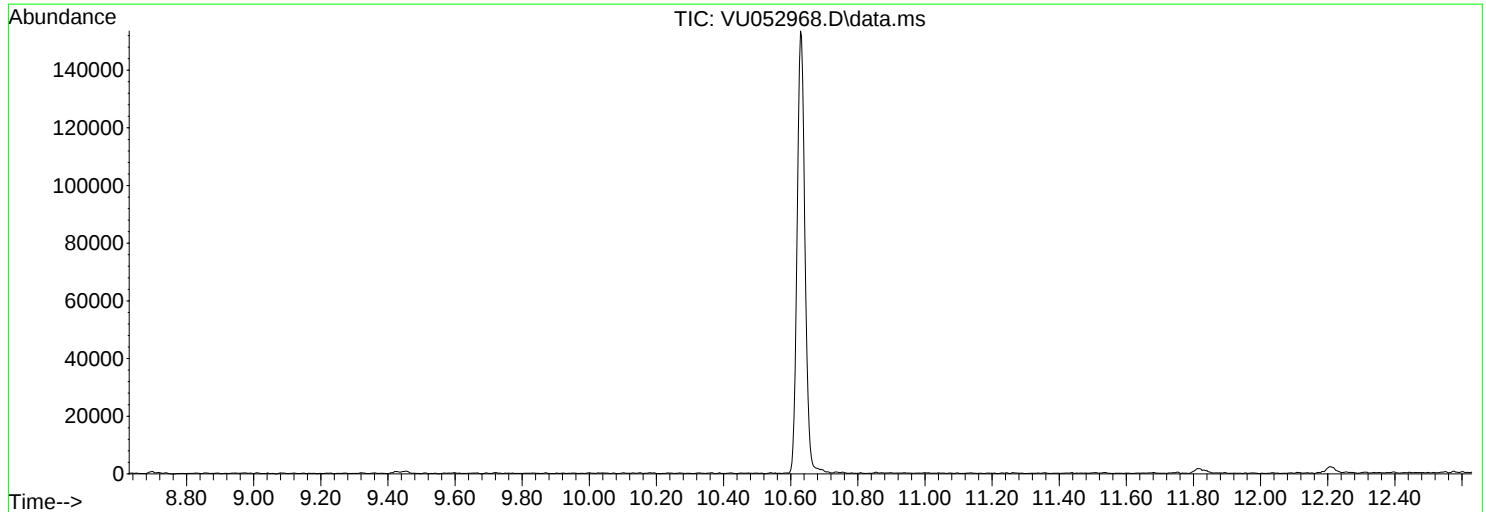

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	4702	PASS
75	95	30	80	46.0	14180	PASS
95	95	100	100	100.0	30845	PASS
96	95	5	9	5.7	1763	PASS
173	174	0.00	2	1.6	434	PASS
174	95	50	120	86.2	26600	PASS
175	174	5	9	8.0	2124	PASS
176	174	95	101	96.6	25707	PASS
177	176	5	9	6.9	1776	PASS

m/z	Abundance
39.70	104.0
44.00	239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB194

m/z	Abundance
35.90	167.0
36.90	1027.0
38.00	655.0
38.90	544.0
44.00	311.0
44.90	158.0
47.00	336.0
47.90	151.0
48.90	1115.0
50.00	4559.0
51.00	1377.0
56.00	359.0
57.10	757.0
59.90	227.0
61.00	1277.0
62.00	1478.0
63.00	1425.0
64.10	371.0
65.10	411.0
68.00	2871.0
69.00	2779.0
69.90	240.0
72.90	1356.0
74.00	4451.0
75.00	13526.0
76.00	1027.0
77.00	187.0
78.90	1350.0
79.90	357.0
80.90	1415.0
81.80	319.0
86.90	1211.0
88.00	1421.0
92.00	1036.0
93.10	1330.0
94.00	3257.0
95.00	30400.0
96.00	1734.0
106.00	101.0
116.90	238.0
118.90	206.0
129.90	134.0
137.00	109.0
140.90	319.0
142.90	509.0
145.00	280.0
171.00	184.0
171.80	351.0
173.10	372.0
174.00	24304.0
175.00	2034.0
176.00	23920.0
176.90	1585.0

Instrument :
MSVOA_U
ClientSampleId :
BFB194

m/z	Abundance
35.90	176.0
37.00	981.0
38.00	680.0
38.90	572.0
40.30	106.0
44.00	414.0
44.90	189.0
47.00	336.0
47.90	183.0
48.90	1178.0
50.00	4838.0
51.00	1391.0
55.00	132.0
55.90	336.0
57.10	782.0
60.00	269.0
61.00	1263.0
62.00	1761.0
63.00	1393.0
64.10	413.0
65.10	388.0
68.00	2962.0
69.00	3149.0
69.90	231.0
72.90	1526.0
74.00	4714.0
75.00	14555.0
76.00	1042.0
77.00	251.0
78.90	1415.0
80.00	397.0
80.90	1366.0
81.90	314.0
86.90	1304.0
88.00	1501.0
92.00	1156.0
93.10	1565.0
94.00	3375.0
95.00	31864.0
96.00	1797.0
106.00	142.0
116.90	260.0
117.90	116.0
118.90	270.0
129.90	139.0
137.00	103.0
140.90	364.0
142.90	593.0
144.90	287.0
171.00	198.0
171.90	440.0
173.00	452.0
174.00	27496.0
175.00	2194.0
176.00	26400.0
176.90	1845.0

Instrument :
MSVOA_U
ClientSampleId :
BFB194

m/z	Abundance
35.90	133.0
37.00	974.0
38.00	717.0
39.00	510.0
44.00	483.0
44.90	187.0
46.90	246.0
47.90	188.0
49.00	1106.0
50.00	4708.0
51.00	1368.0
55.00	160.0
56.00	270.0
57.00	692.0
60.00	304.0
61.00	1223.0
62.00	1824.0
63.00	1343.0
64.00	424.0
65.00	385.0
68.00	2754.0
69.00	3050.0
70.00	192.0
72.90	1503.0
74.00	4674.0
75.00	14459.0
76.00	1039.0
77.00	297.0
78.90	1435.0
80.00	417.0
80.90	1287.0
81.90	274.0
87.00	1378.0
88.00	1341.0
92.00	1121.0
93.00	1442.0
94.00	3186.0
95.00	30272.0
96.00	1757.0
106.00	150.0
117.00	278.0
117.90	118.0
118.90	310.0
128.00	102.0
129.90	134.0
140.90	335.0
142.90	653.0
144.80	304.0
147.70	125.0
171.00	176.0
172.00	430.0
173.00	478.0
174.00	28000.0
175.00	2143.0
176.00	26800.0
176.90	1899.0

Instrument :
MSVOA_U
ClientSampleId :
BFB194