

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
 Data File : VU057813.D
 Acq On : 06 Feb 2024 10:11
 Operator : MD/SY
 Sample : VU0206WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0206WBL01

Quant Time: Feb 07 02:58:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 06 02:05:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	42729	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	14083	0.898	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	11842	0.854	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020624\
Data File : VU057813.D
Acq On : 06 Feb 2024 10:11
Operator : MD/SY
Sample : VU0206WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0206WBL01

Quant Time: Feb 07 02:58:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U020524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 06 02:05:40 2024
Response via : Initial Calibration




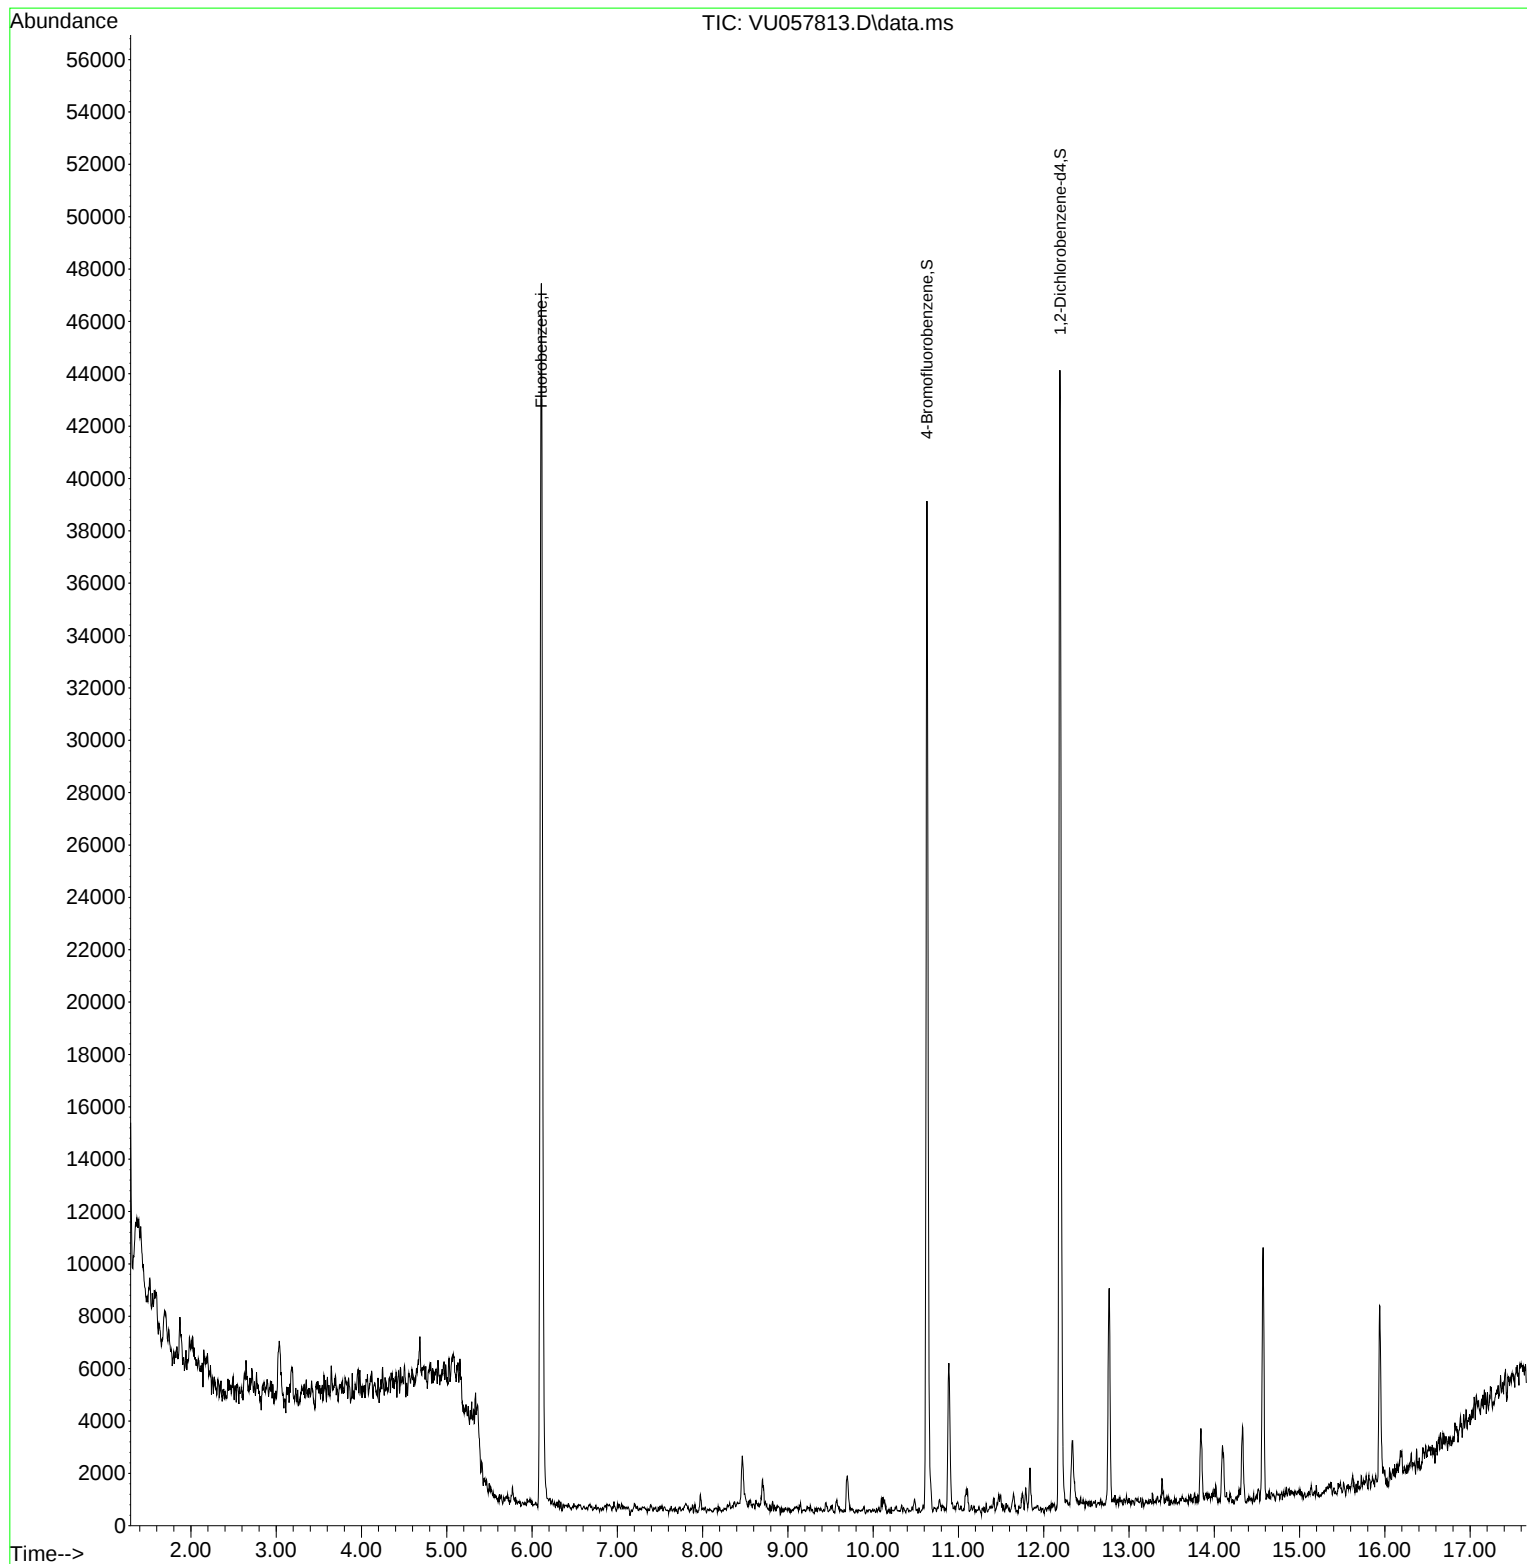


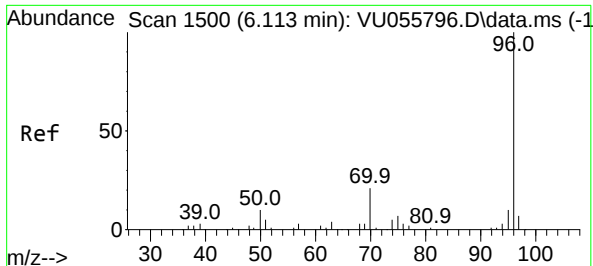

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1499
Delta R.T. 0.007 min
Lab File: VU057813.D
Acq: 06 Feb 2024 10:11




Instrument :
MSVOA_U
ClientSampleId :
VU0206WBL01


Tgt Ion: 96	Resp: 42729
Ion Ratio	Lower Upper
96 100	
70 20.7	16.5 24.7
95 9.2	7.4 11.0
97 6.3	0.0 0.0

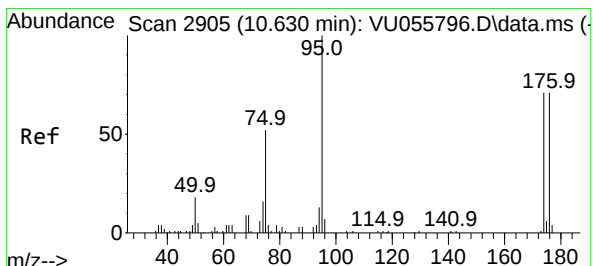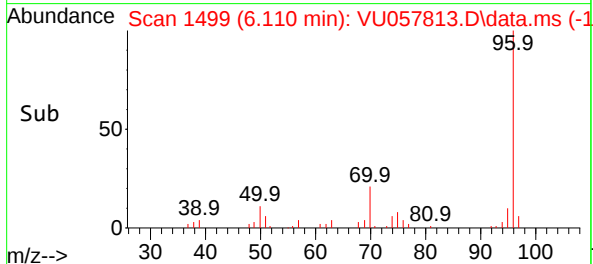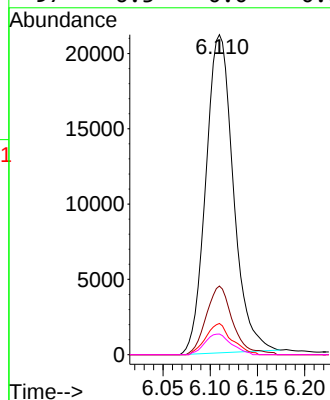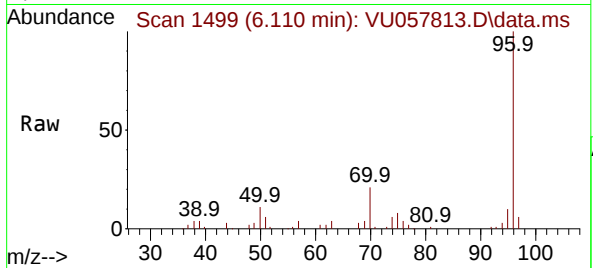

#57
4-Bromofluorobenzene
Concen: 0.898 ug/l
RT: 10.630 min Scan# 2905
Delta R.T. 0.000 min
Lab File: VU057813.D
Acq: 06 Feb 2024 10:11


Tgt Ion: 95	Resp: 14083
Ion Ratio	Lower Upper
95 100	
174 73.2	63.3 94.9
176 70.9	59.3 88.9

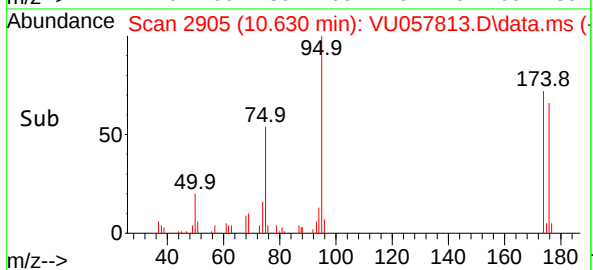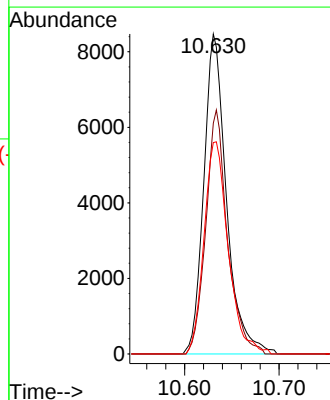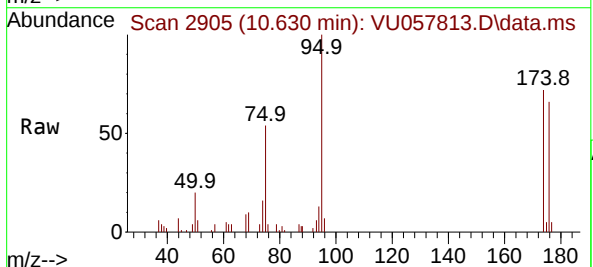

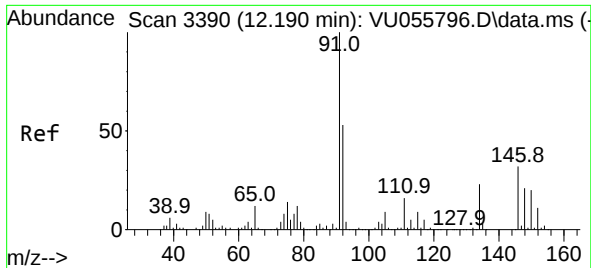

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.854 ug/l
 RT: 12.193 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU057813.D
 Acq: 06 Feb 2024 10:11

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0206WBL01

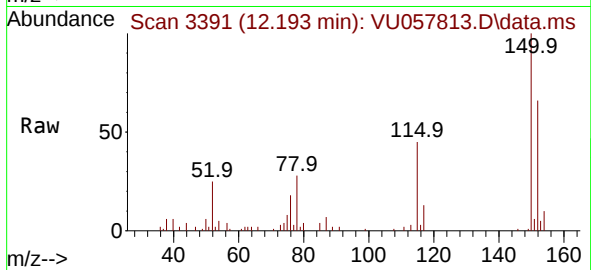

Tgt Ion:	152	Resp:	11842
Ion Ratio	Lower	Upper	
152	100		
115	71.3	0.0	308.8
150	161.5	0.0	635.0

